
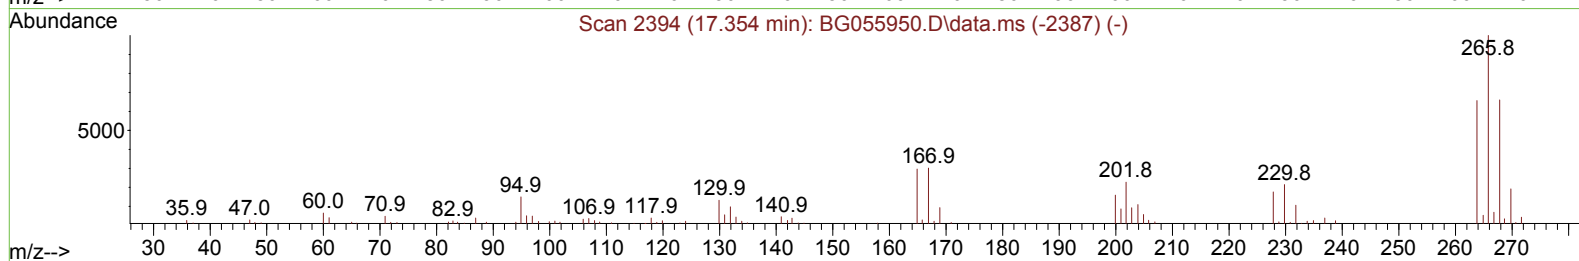
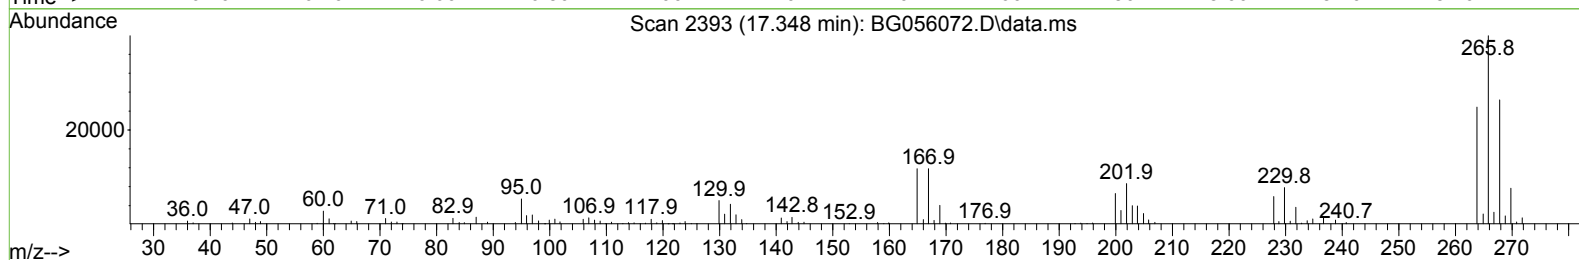


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122322\
Data File : BG056072.D
Acq On : 23 Dec 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 02:31:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

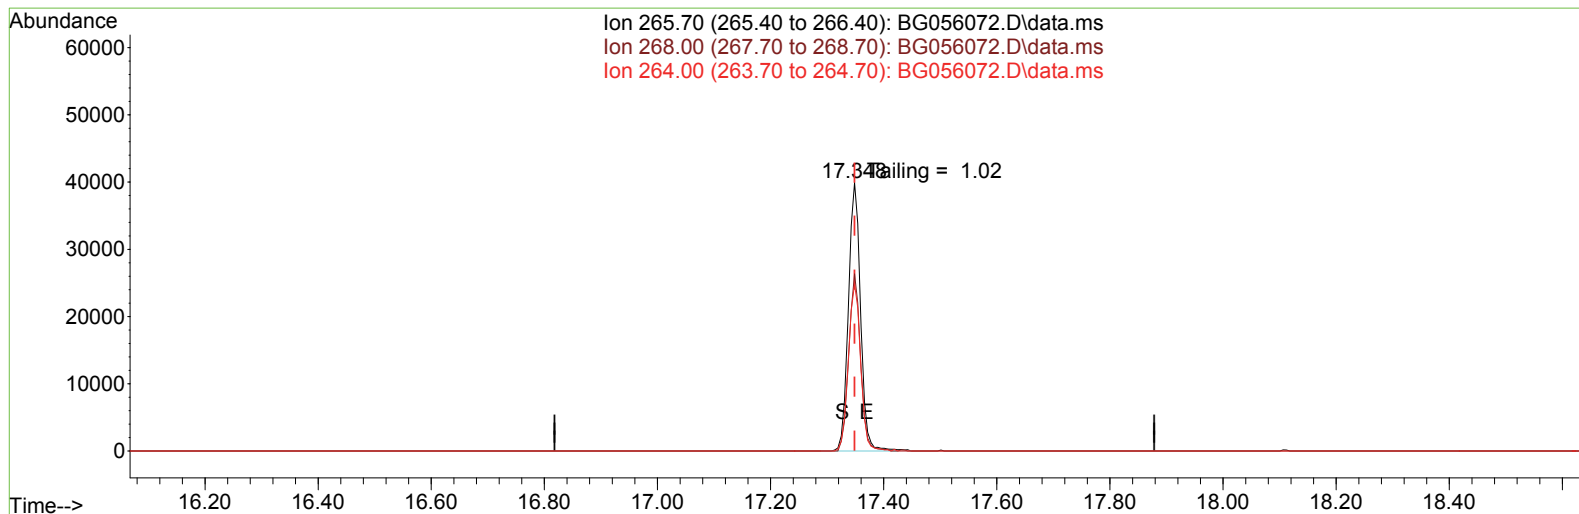

TIC: BG056072.D\data.ms

(70) Pentachlorophenol (C)




17.348min (-0.000) 25794.65 ng

response 59886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	66.01
264.00	65.70	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122322\
Data File : BG056072.D
Acq On : 23 Dec 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 02:31:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

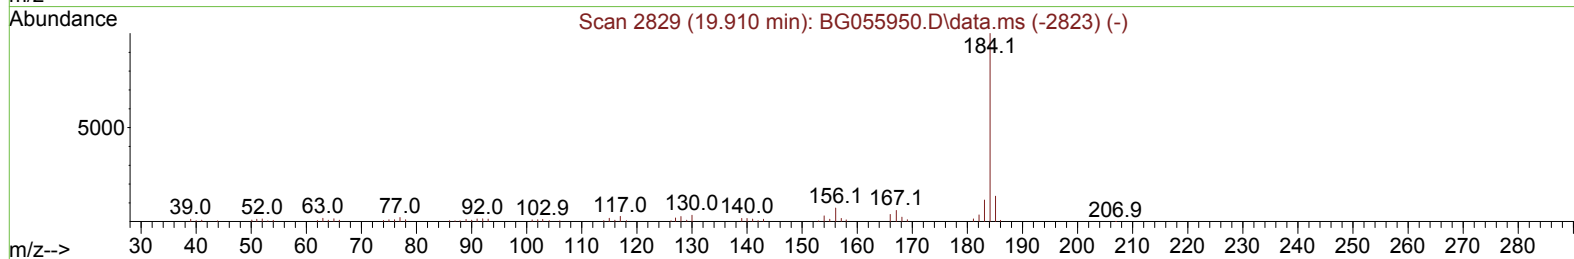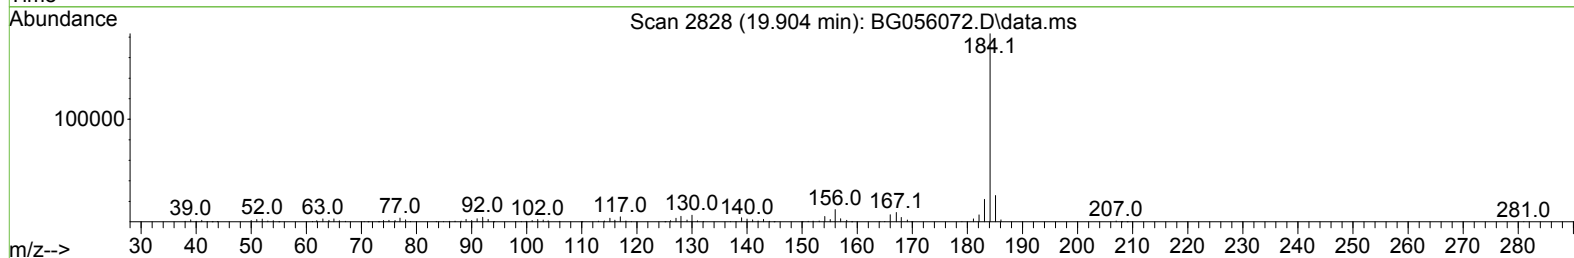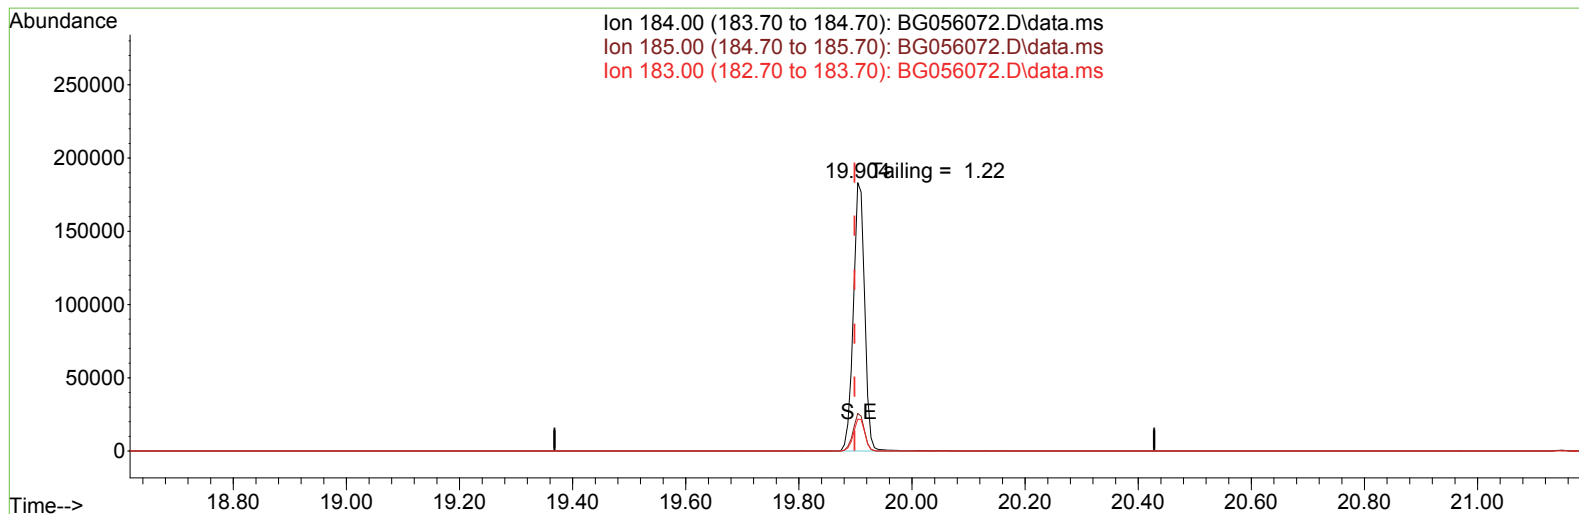

TIC: BG056072.D\data.ms

(77) Benzidine

19.904min (+ 0.006) 16631.61 ng

response 254401

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	11.50	11.96
0.00	0.00	0.00