
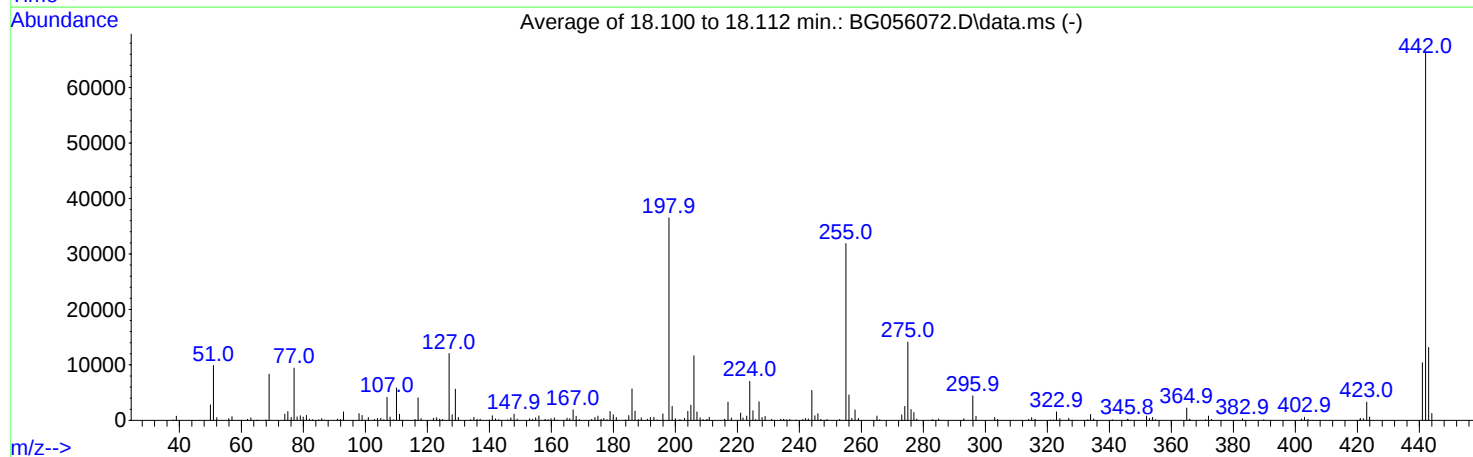


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122322\
 Data File : BG056072.D
 Acq On : 23 Dec 2022 9:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 05:09:54 2022

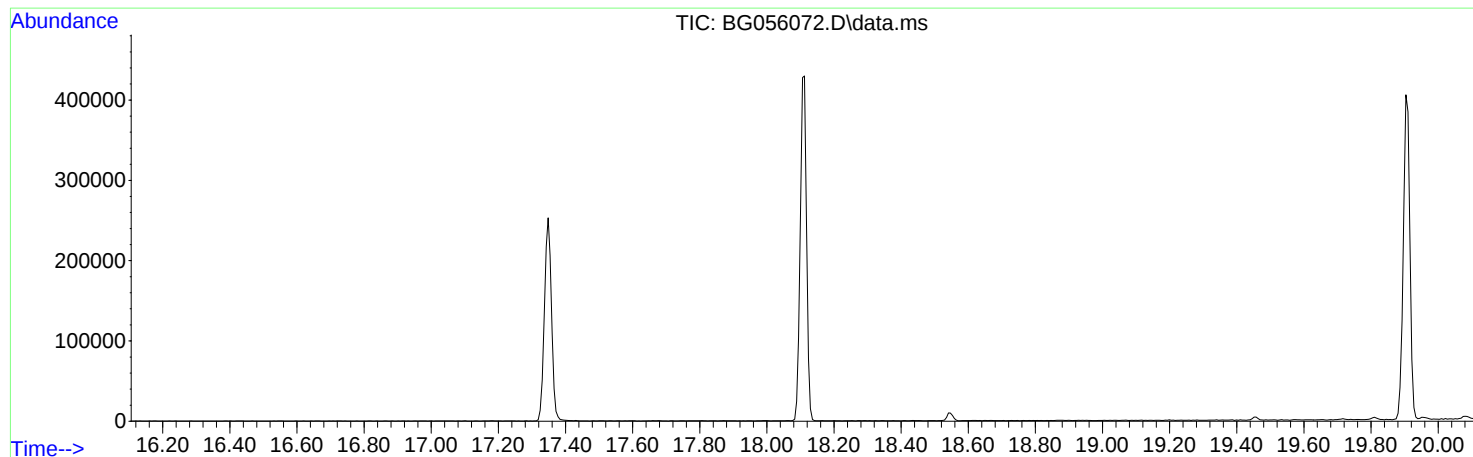




AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	9895	PASS
68	69	0.00	2	0.9	77	PASS
69	198	0.00	100	22.9	8355	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.1	12075	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36533	PASS
199	198	5	9	6.9	2536	PASS
275	198	10	60	38.6	14108	PASS
365	198	1	100	6.1	2235	PASS
441	198	0.01	100	28.4	10384	PASS
442	442	50	100	100.0	66323	PASS
443	442	15	24	19.8	13159	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122322\
Data File : BG056072.D
Acq On : 23 Dec 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 24 02:31:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

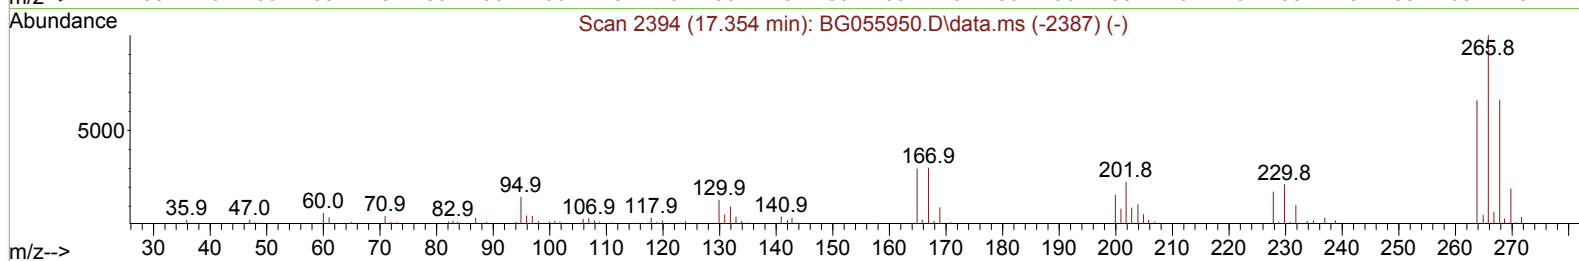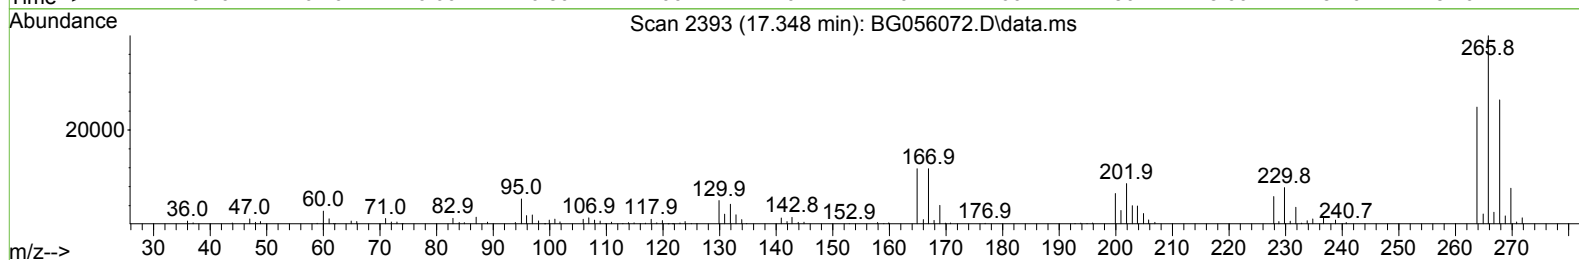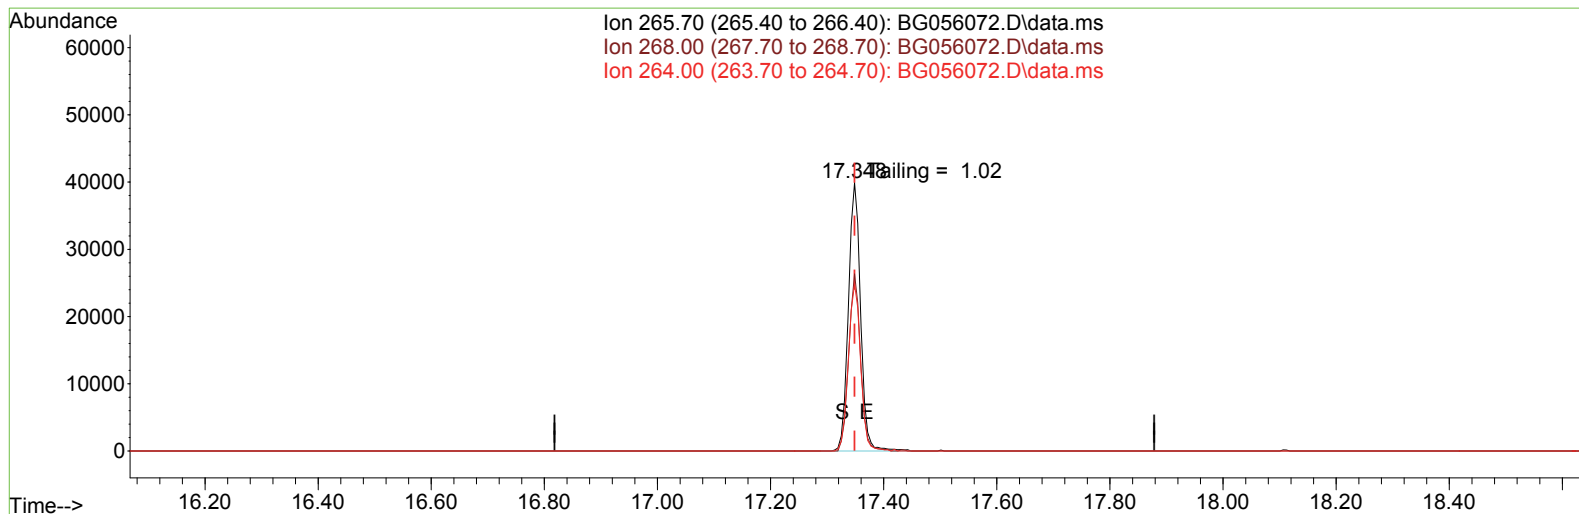

TIC: BG056072.D\data.ms

(70) Pentachlorophenol (C)

17.348min (-0.000) 25794.65 ng




response 59886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	66.01
264.00	65.70	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122322\
Data File : BG056072.D
Acq On : 23 Dec 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 24 02:31:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

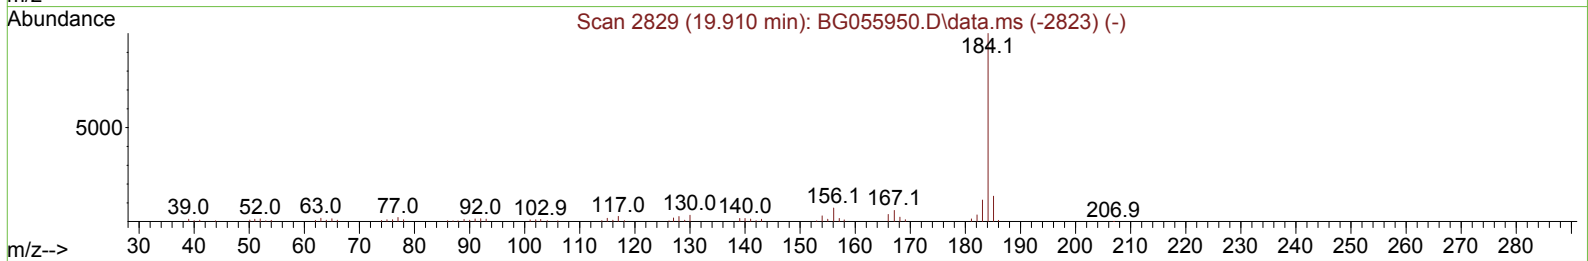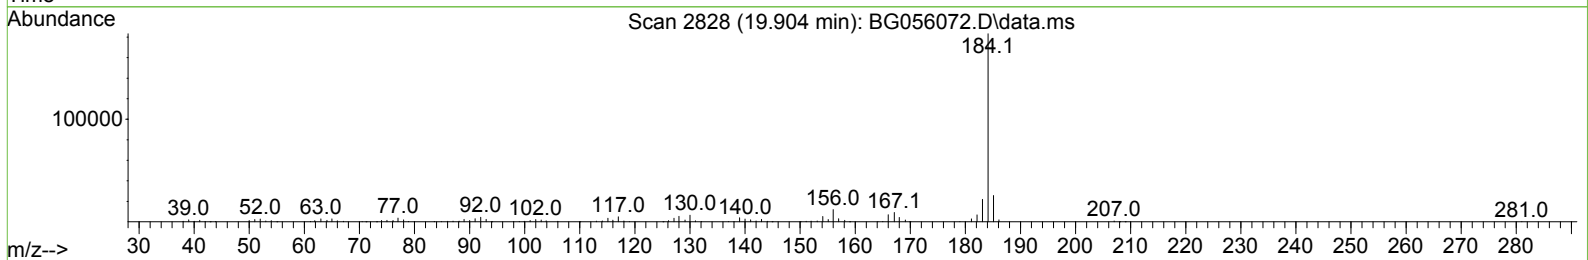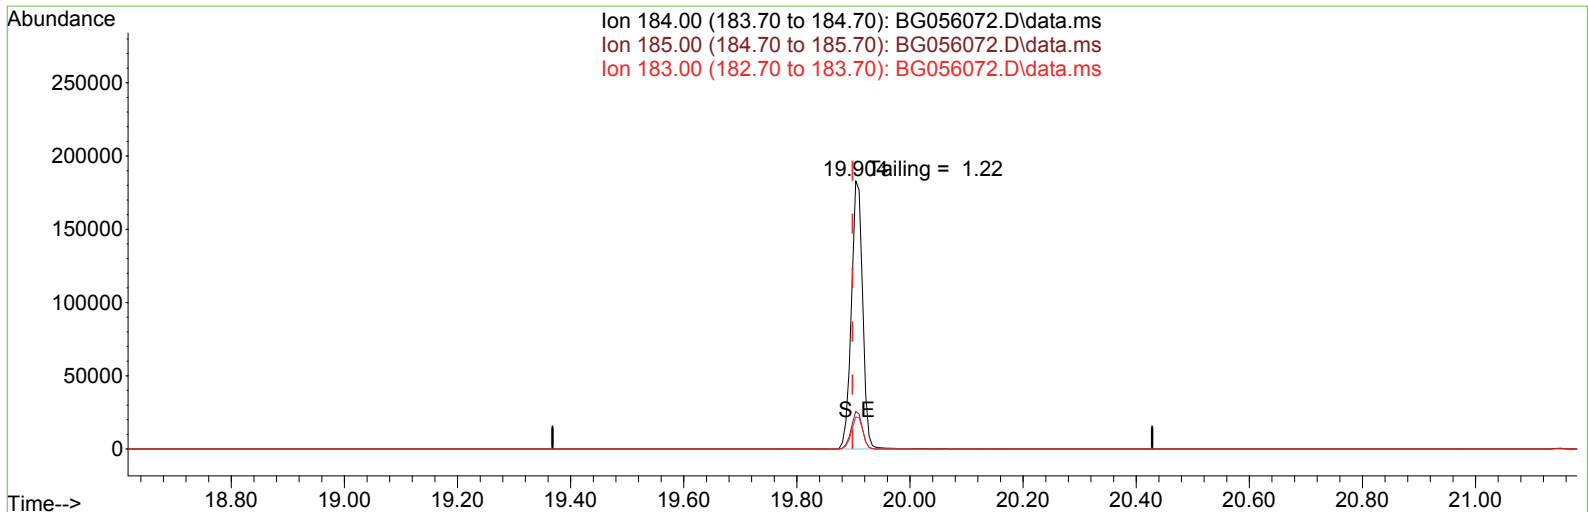

TIC: BG056072.D\data.ms

(77) Benzidine

19.904min (+ 0.006) 16631.61 ng

response 254401

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	11.50	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/23/2022	BNA_G	BG056072.D
Compound Name	Response	Retention Time
DDT	144318	21.15
DDD	4311	20.686
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4311	148629	2.90

Instrument :
BNA_G
ClientSampleId :
DFTPP