

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
 Data File : BG063825.D
 Acq On : 24 Dec 2024 18:36
 Operator : RC/JU
 Sample : P5333-16
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E2918

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.670	95	99	109	rBV	119109	205830	8.46%	0.845%
2	3.793	118	120	122	rBV3	10147	10338	0.42%	0.042%
3	4.298	204	206	208	rBV3	9649	7781	0.32%	0.032%
4	4.669	267	269	272	rVB2	8424	6645	0.27%	0.027%
5	5.450	400	402	405	rBV3	6120	7544	0.31%	0.031%
6	5.797	458	461	462	rBV2	9386	8201	0.34%	0.034%
7	6.872	643	644	647	rBV	7040	6934	0.28%	0.028%
8	6.983	658	663	675	rVB	257691	495015	20.34%	2.033%
9	7.130	682	688	696	rVB	215995	365552	15.02%	1.501%
10	7.336	717	723	729	rBV2	254467	420432	17.28%	1.726%
11	7.571	761	763	766	rBV2	6175	6645	0.27%	0.027%
12	7.694	781	784	787	rBV3	7382	10758	0.44%	0.044%
13	7.800	795	802	809	rVB	376690	634355	26.07%	2.605%
14	8.211	870	872	876	rBV3	7278	8971	0.37%	0.037%
15	8.517	917	924	934	rBV2	278895	497359	20.44%	2.042%
16	8.952	992	998	1006	rBV	264782	484618	19.91%	1.990%
17	9.110	1022	1025	1026	rBV3	8187	6874	0.28%	0.028%
18	9.128	1026	1028	1030	rVB2	8884	6386	0.26%	0.026%
19	9.228	1042	1045	1047	rBV2	6978	7986	0.33%	0.033%
20	9.375	1067	1070	1076	rVB5	9573	12661	0.52%	0.052%
21	9.510	1088	1093	1100	rBV4	28688	53028	2.18%	0.218%
22	9.674	1113	1121	1130	rVV2	228396	426797	17.54%	1.752%
23	9.974	1170	1172	1176	rVB	5142	6342	0.26%	0.026%
24	10.092	1189	1192	1195	rBV3	6762	10005	0.41%	0.041%
25	10.221	1205	1214	1225	rBV2	341739	658144	27.05%	2.702%
26	10.491	1257	1260	1264	rBV2	6461	10095	0.41%	0.041%
27	10.585	1269	1276	1282	rBV	567412	1007111	41.39%	4.135%
28	10.726	1293	1300	1308	rBV2	235584	465939	19.15%	1.913%
29	10.973	1339	1342	1345	rVB2	6491	7401	0.30%	0.030%
30	11.126	1362	1368	1373	rVB2	16677	33956	1.40%	0.139%
31	11.419	1416	1418	1421	rBV2	7931	7203	0.30%	0.030%
32	11.760	1469	1476	1477	rBV3	5931	10013	0.41%	0.041%
33	11.954	1507	1509	1511	rBV3	5639	6358	0.26%	0.026%
34	12.007	1514	1518	1523	rVV5	12442	23500	0.97%	0.096%
35	12.048	1523	1525	1529	rVB2	6400	7097	0.29%	0.029%
36	12.183	1546	1548	1551	rVV3	7219	7339	0.30%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
 Data File : BG063825.D
 Acq On : 24 Dec 2024 18:36
 Operator : RC/JU
 Sample : P5333-16
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E2918

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

37	12.254	1555	1560	1565	rBV5	18000	36159	1.49%	0.148%
38	12.471	1596	1597	1600	rVV3	10022	10425	0.43%	0.043%
39	12.965	1678	1681	1682	rBV2	7051	8777	0.36%	0.036%
40	13.264	1729	1732	1738	rVV4	22919	33464	1.38%	0.137%
41	13.317	1738	1741	1743	rVB2	6697	6423	0.26%	0.026%
42	13.423	1752	1759	1762	rBV3	20101	34708	1.43%	0.143%
43	13.599	1787	1789	1792	rBV2	9229	8735	0.36%	0.036%
44	13.752	1814	1815	1816	rBV	13966	6402	0.26%	0.026%
45	13.846	1822	1831	1836	rBV	727086	1058483	43.50%	4.346%
46	13.887	1836	1838	1843	rVB2	28563	37476	1.54%	0.154%
47	13.969	1848	1852	1855	rBV5	5928	9458	0.39%	0.039%
48	13.993	1855	1856	1860	rVB2	12136	9139	0.38%	0.038%
49	14.128	1873	1879	1890	rBV2	683714	1097648	45.11%	4.507%
50	14.310	1909	1910	1912	rBV2	8037	6960	0.29%	0.029%
51	14.340	1912	1915	1919	rVB5	13123	19963	0.82%	0.082%
52	14.439	1924	1932	1939	rBV	1053940	1615587	66.39%	6.634%
53	14.492	1939	1941	1946	rBV5	8166	10641	0.44%	0.044%
54	14.598	1957	1959	1963	rVB2	9329	9533	0.39%	0.039%
55	14.639	1963	1966	1967	rBV2	6601	6968	0.29%	0.029%
56	14.680	1967	1973	1981	rBV2	116364	246963	10.15%	1.014%
57	14.815	1993	1996	1997	rBV3	8129	9800	0.40%	0.040%
58	14.904	2008	2011	2012	rBV2	7889	9467	0.39%	0.039%
59	15.068	2036	2039	2042	rVB4	11246	14080	0.58%	0.058%
60	15.103	2042	2045	2047	rBV3	10055	8834	0.36%	0.036%
61	15.180	2056	2058	2061	rVB2	10969	9338	0.38%	0.038%
62	15.238	2061	2068	2070	rBV5	13644	27348	1.12%	0.112%
63	15.291	2073	2077	2081	rBV5	17259	22786	0.94%	0.094%
64	15.356	2085	2088	2091	rVB	6528	6673	0.27%	0.027%
65	15.438	2095	2102	2107	rBV	823993	1260538	51.80%	5.176%
66	15.573	2120	2125	2132	rBV2	103212	169092	6.95%	0.694%
67	15.797	2158	2163	2171	rVB	801648	1164050	47.83%	4.780%
68	16.014	2198	2200	2203	rBV4	7140	8163	0.34%	0.034%
69	16.155	2220	2224	2225	rBV2	24214	23696	0.97%	0.097%
70	16.255	2239	2241	2244	rBV4	5069	6273	0.26%	0.026%
71	16.361	2255	2259	2266	rVV	127215	197960	8.13%	0.813%
72	16.472	2275	2278	2279	rVV3	8024	7484	0.31%	0.031%
73	16.502	2281	2283	2286	rVV4	12349	11261	0.46%	0.046%
74	16.543	2288	2290	2294	rVB3	11982	14289	0.59%	0.059%
75	16.649	2306	2308	2313	rBV5	8932	12353	0.51%	0.051%
76	16.707	2315	2318	2319	rBV3	6564	7911	0.33%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
 Data File : BG063825.D
 Acq On : 24 Dec 2024 18:36
 Operator : RC/JU
 Sample : P5333-16
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E2918

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

77	16.731	2320	2322	2324	rVV3	9889	7761	0.32%	0.032%
78	16.772	2326	2329	2331	rVV3	8227	7088	0.29%	0.029%
79	16.848	2339	2342	2350	rVB10	20232	38719	1.59%	0.159%
80	16.913	2350	2353	2354	rBV2	10835	12056	0.50%	0.050%
81	16.948	2356	2359	2363	rVB4	26354	26203	1.08%	0.108%
82	17.101	2383	2385	2390	rVB6	11362	12812	0.53%	0.053%
83	17.189	2394	2400	2405	rBV2	1394499	2103432	86.44%	8.637%
84	17.289	2411	2417	2426	rVB	929655	1349030	55.44%	5.539%
85	17.436	2440	2442	2444	rBV3	10087	6203	0.25%	0.025%
86	17.689	2483	2485	2489	rVB5	20587	23120	0.95%	0.095%
87	17.853	2509	2513	2514	rBV4	11256	12288	0.50%	0.050%
88	18.035	2540	2544	2547	rBV6	36257	65619	2.70%	0.269%
89	18.070	2547	2550	2551	rBV	25745	27027	1.11%	0.111%
90	18.094	2551	2554	2557	rBV3	51068	81863	3.36%	0.336%
91	18.258	2579	2582	2587	rVB4	35020	52450	2.16%	0.215%
92	18.382	2600	2603	2607	rBV5	48291	75460	3.10%	0.310%
93	18.817	2674	2677	2682	rVB7	23849	33406	1.37%	0.137%
94	18.993	2703	2707	2710	rBV2	55584	88928	3.65%	0.365%
95	19.251	2747	2751	2758	rVB	209803	307502	12.64%	1.263%
96	19.586	2803	2808	2813	rBV	904403	1442978	59.30%	5.925%
97	21.102	3063	3066	3077	rVB6	144447	271170	11.14%	1.113%
98	21.437	3117	3123	3128	rBV	1436765	2433501	100.00%	9.992%
99	24.240	3596	3600	3606	rVB2	206672	421082	17.30%	1.729%
100	24.451	3628	3636	3645	rBV	846488	2237490	91.95%	9.187%


Sum of corrected areas: 24353709

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
Data File : BG063825.D
Acq On : 24 Dec 2024 18:36
Operator : RC/JU
Sample : P5333-16
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

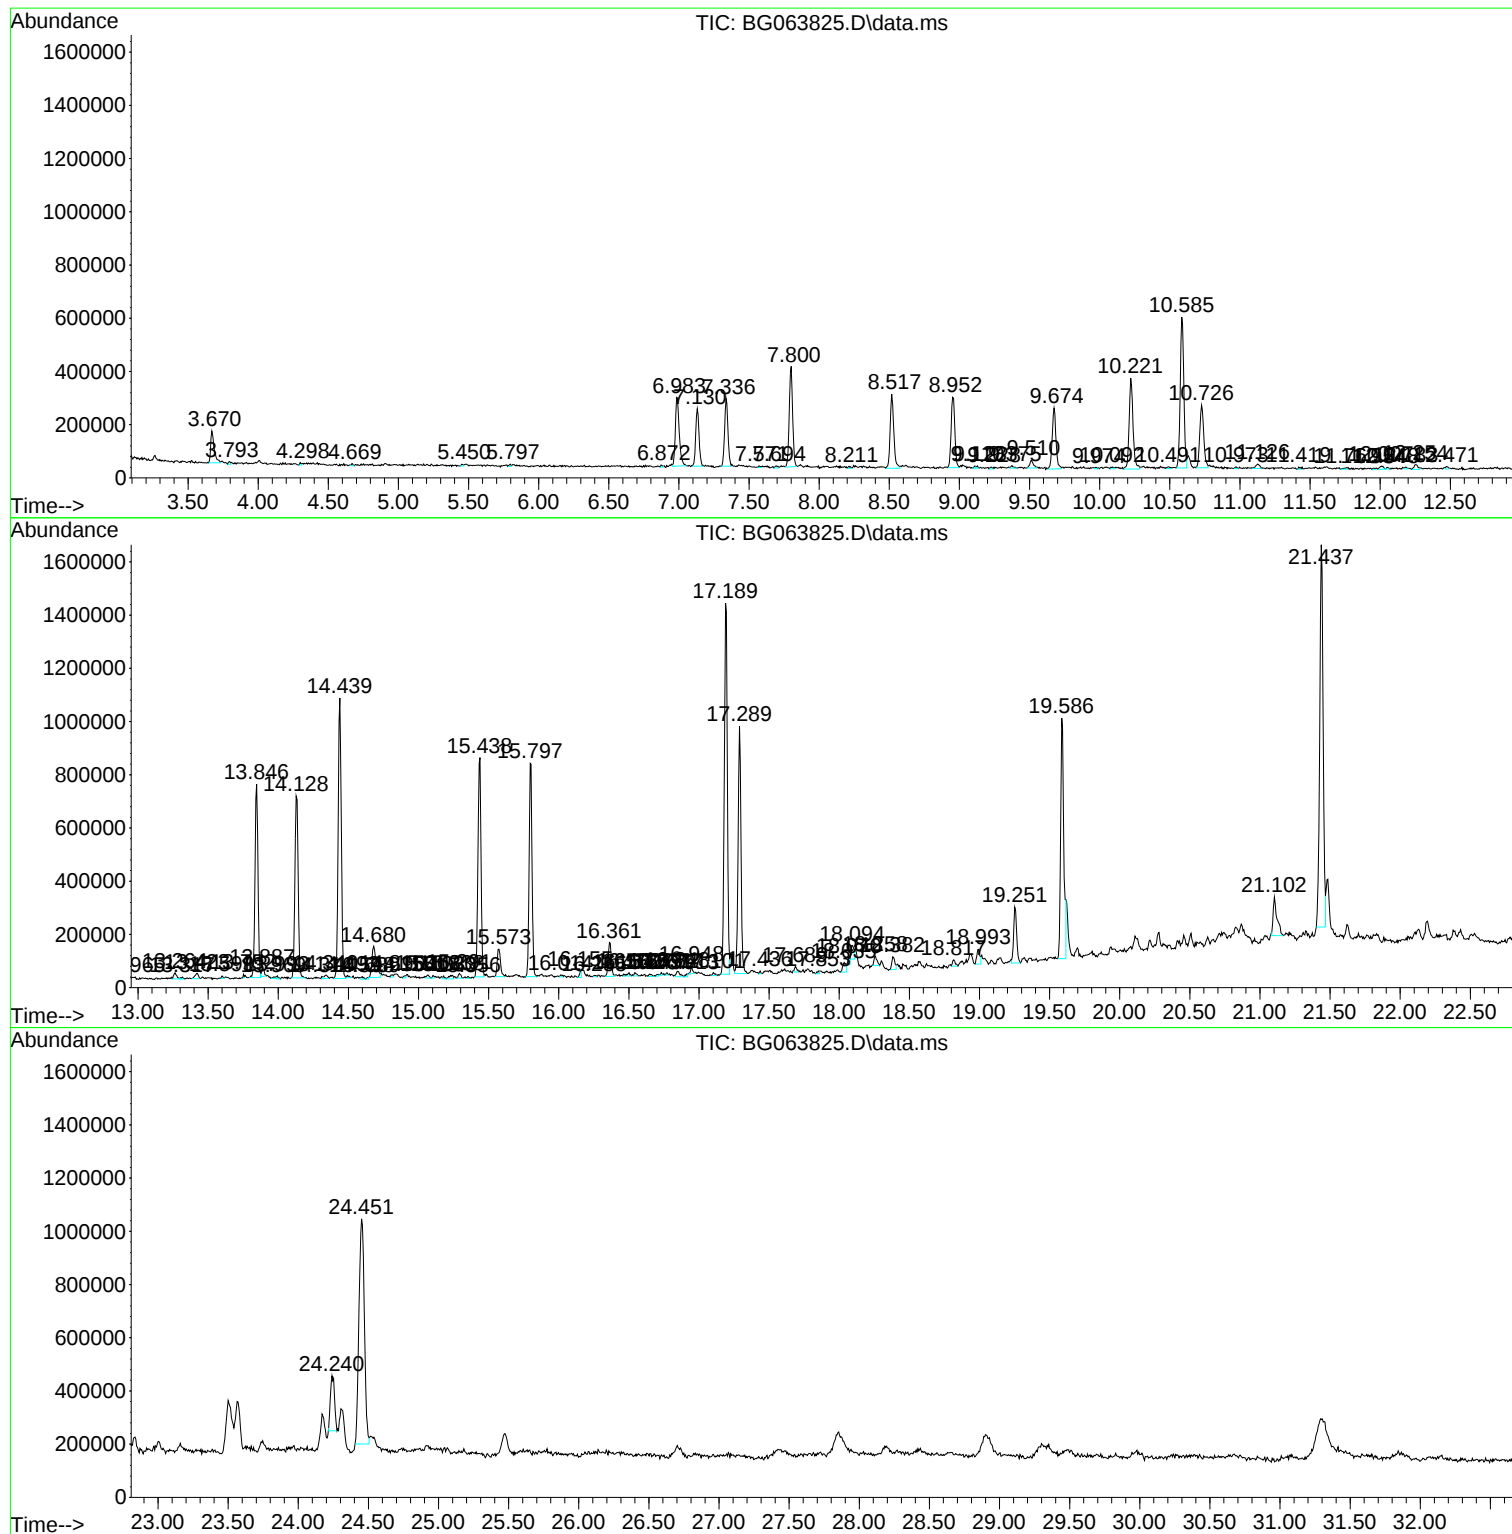

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
Data File : BG063825.D
Acq On : 24 Dec 2024 18:36
Operator : RC/JU
Sample : P5333-16
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2918










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.797	14.41 ng/ul	1164050	Acenaphthene-d10	14.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			2-Phenyl-4-ethylidene-2-oxazolin...	187	C11H9NO2	037791-41-6	53

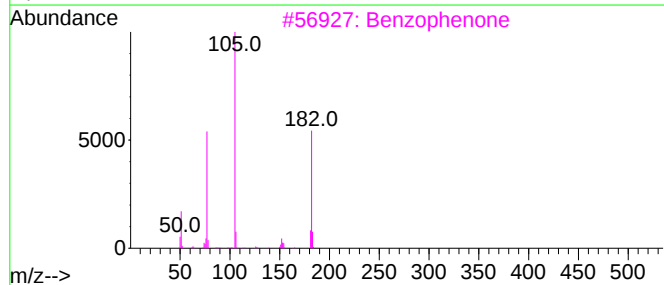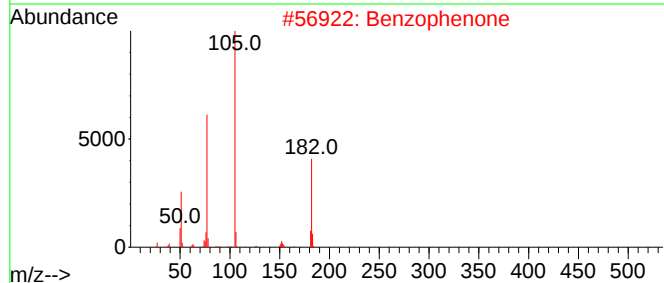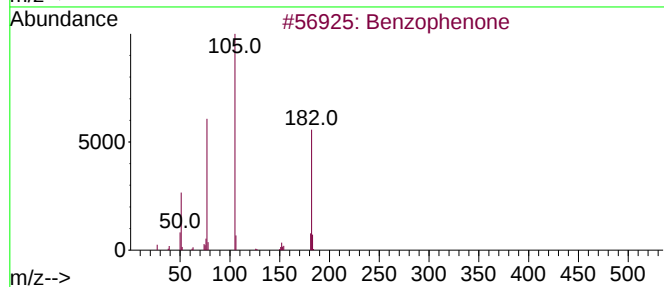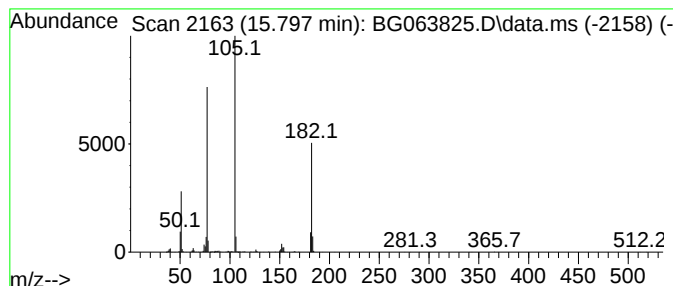

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
Data File : BG063825.D
Acq On : 24 Dec 2024 18:36
Operator : RC/JU
Sample : P5333-16
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2918










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.102	2.23 ng/ul	271170	Chrysene-d12	21.437

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Octadecene	252	C18H36	000112-88-9	92
2			1-Octadecene	252	C18H36	000112-88-9	92
3			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
4			3-Octadecene, (E)-	252	C18H36	007206-19-1	87
5			Cetene	224	C16H32	000629-73-2	78

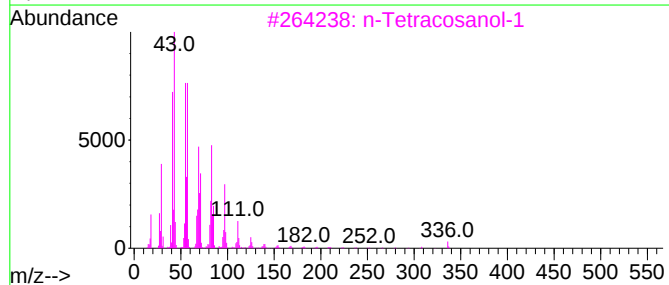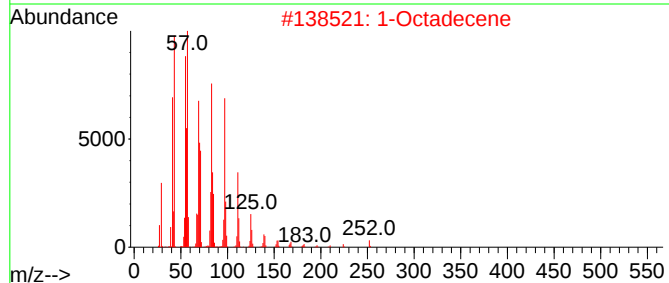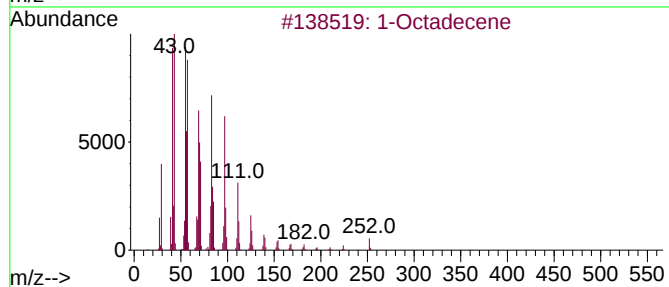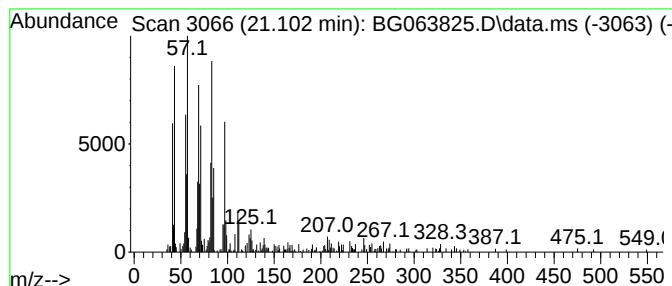

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122324\
Data File : BG063825.D
Acq On : 24 Dec 2024 18:36
Operator : RC/JU
Sample : P5333-16
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.797	14.4	ng/u1	1164050	3	14.439	1615590	20.0
(DEL) Alkane: S...	21.102	2.2	ng/u1	271170	5	21.437	2433500	20.0