

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020478.D
 Acq On : 24 Dec 2015 18:28
 Operator : UM/SJ
 Sample : G4803-12RX
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04C0RX

Quant Time: Dec 25 02:22:54 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 02:19:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	16740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	68469	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	46870	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	121220	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	164300	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	159590	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	238	0.78	ng/uL	0.00
5) Phenol-d5	7.23	99	7060	5.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	17960	22.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	20301	19.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	13655	12.08	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	12255	22.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	14264	23.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.51	165	25531	21.62	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	93629	24.24	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	100576	22.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	2399	3.72	ng/ul	0.00
58) Fluorene-d10	15.70	176	78486	22.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	15074	18.76	ng/ul	0.00
71) Anthracene-d10	17.55	188	128728	22.67	ng/ul	0.00
79) Pyrene-d10	19.84	212	166538	23.41	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	174345	21.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.16	163	17598	4.48	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020478.D
Acq On : 24 Dec 2015 18:28
Operator : UM/SJ
Sample : G4803-12RX
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04C0RX

Quant Time: Dec 25 02:22:54 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 02:19:33 2015
Response via : Initial Calibration

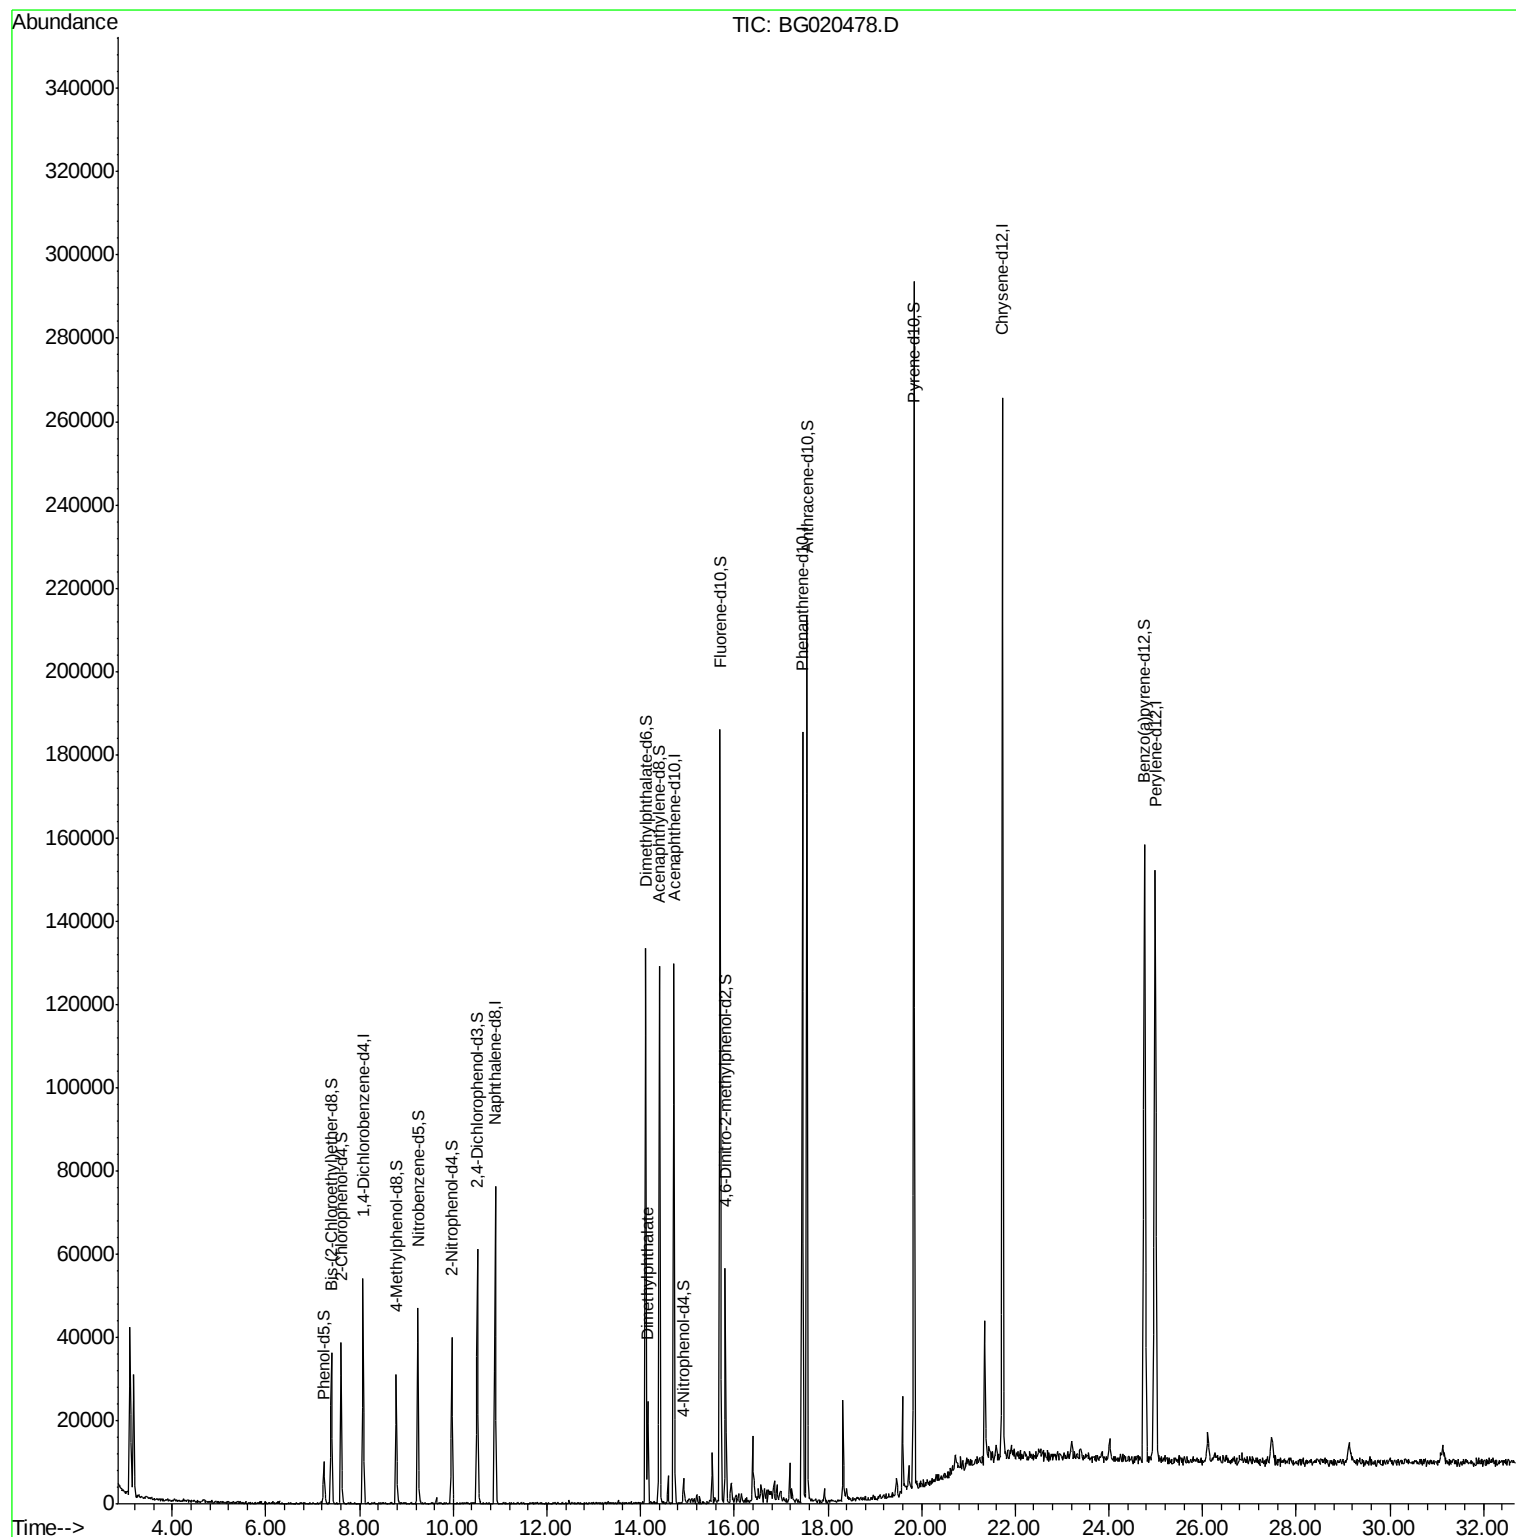

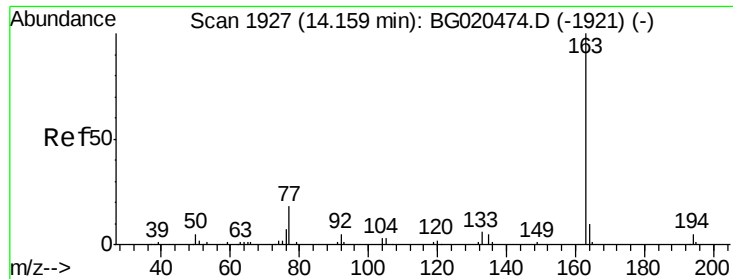

#45

Dimethylphthalate

Concen: 4.48 ng/ul

RT: 14.16 min Scan# 1926

Delta R.T. -0.00 min

Lab File: BG020478.D


Acq: 24 Dec 2015 18:28

Instrument :

BNA_G

ClientSampleId :

C04C0RX

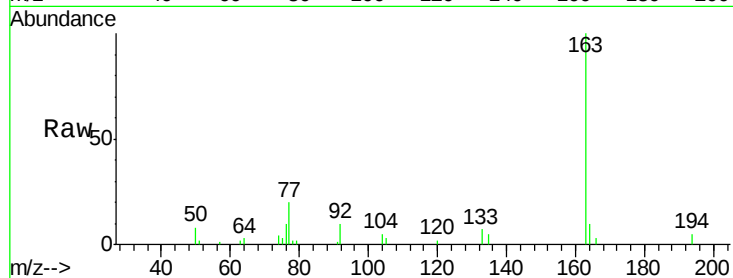


Tgt Ion:163 Resp: 17598

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 10.4 7.7 11.5

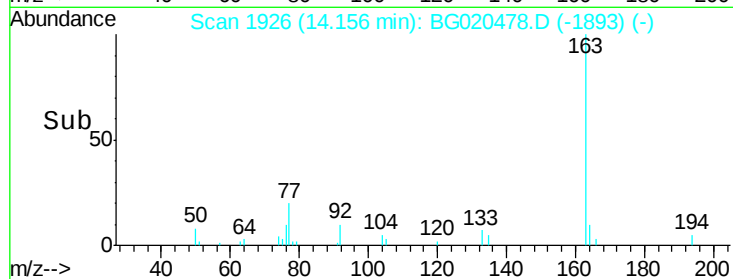

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

