

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020480.D
 Acq On : 24 Dec 2015 19:48
 Operator : UM/SJ
 Sample : PB87462BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK62

Quant Time: Dec 25 02:23:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 02:19:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	13620	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	59141	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	44280	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	117096	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	158013	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	152501	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	1919	7.77	ng/uL	0.00
5) Phenol-d5	7.24	99	40524	37.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	26120	40.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	33969	40.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.78	113	37167	40.42	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	18404	39.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	22064	41.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	39089	38.32	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	51148	43.89	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	155163	42.51	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	169406	40.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	23286	38.27	ng/ul	0.00
58) Fluorene-d10	15.70	176	133587	40.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	28506	36.73	ng/ul	0.00
71) Anthracene-d10	17.56	188	234505	42.76	ng/ul	0.00
79) Pyrene-d10	19.84	212	298242	43.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	345964	44.87	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.78	70	784	1.05 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020480.D
Acq On : 24 Dec 2015 19:48
Operator : UM/SJ
Sample : PB87462BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK62

Quant Time: Dec 25 02:23:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 02:19:33 2015
Response via : Initial Calibration

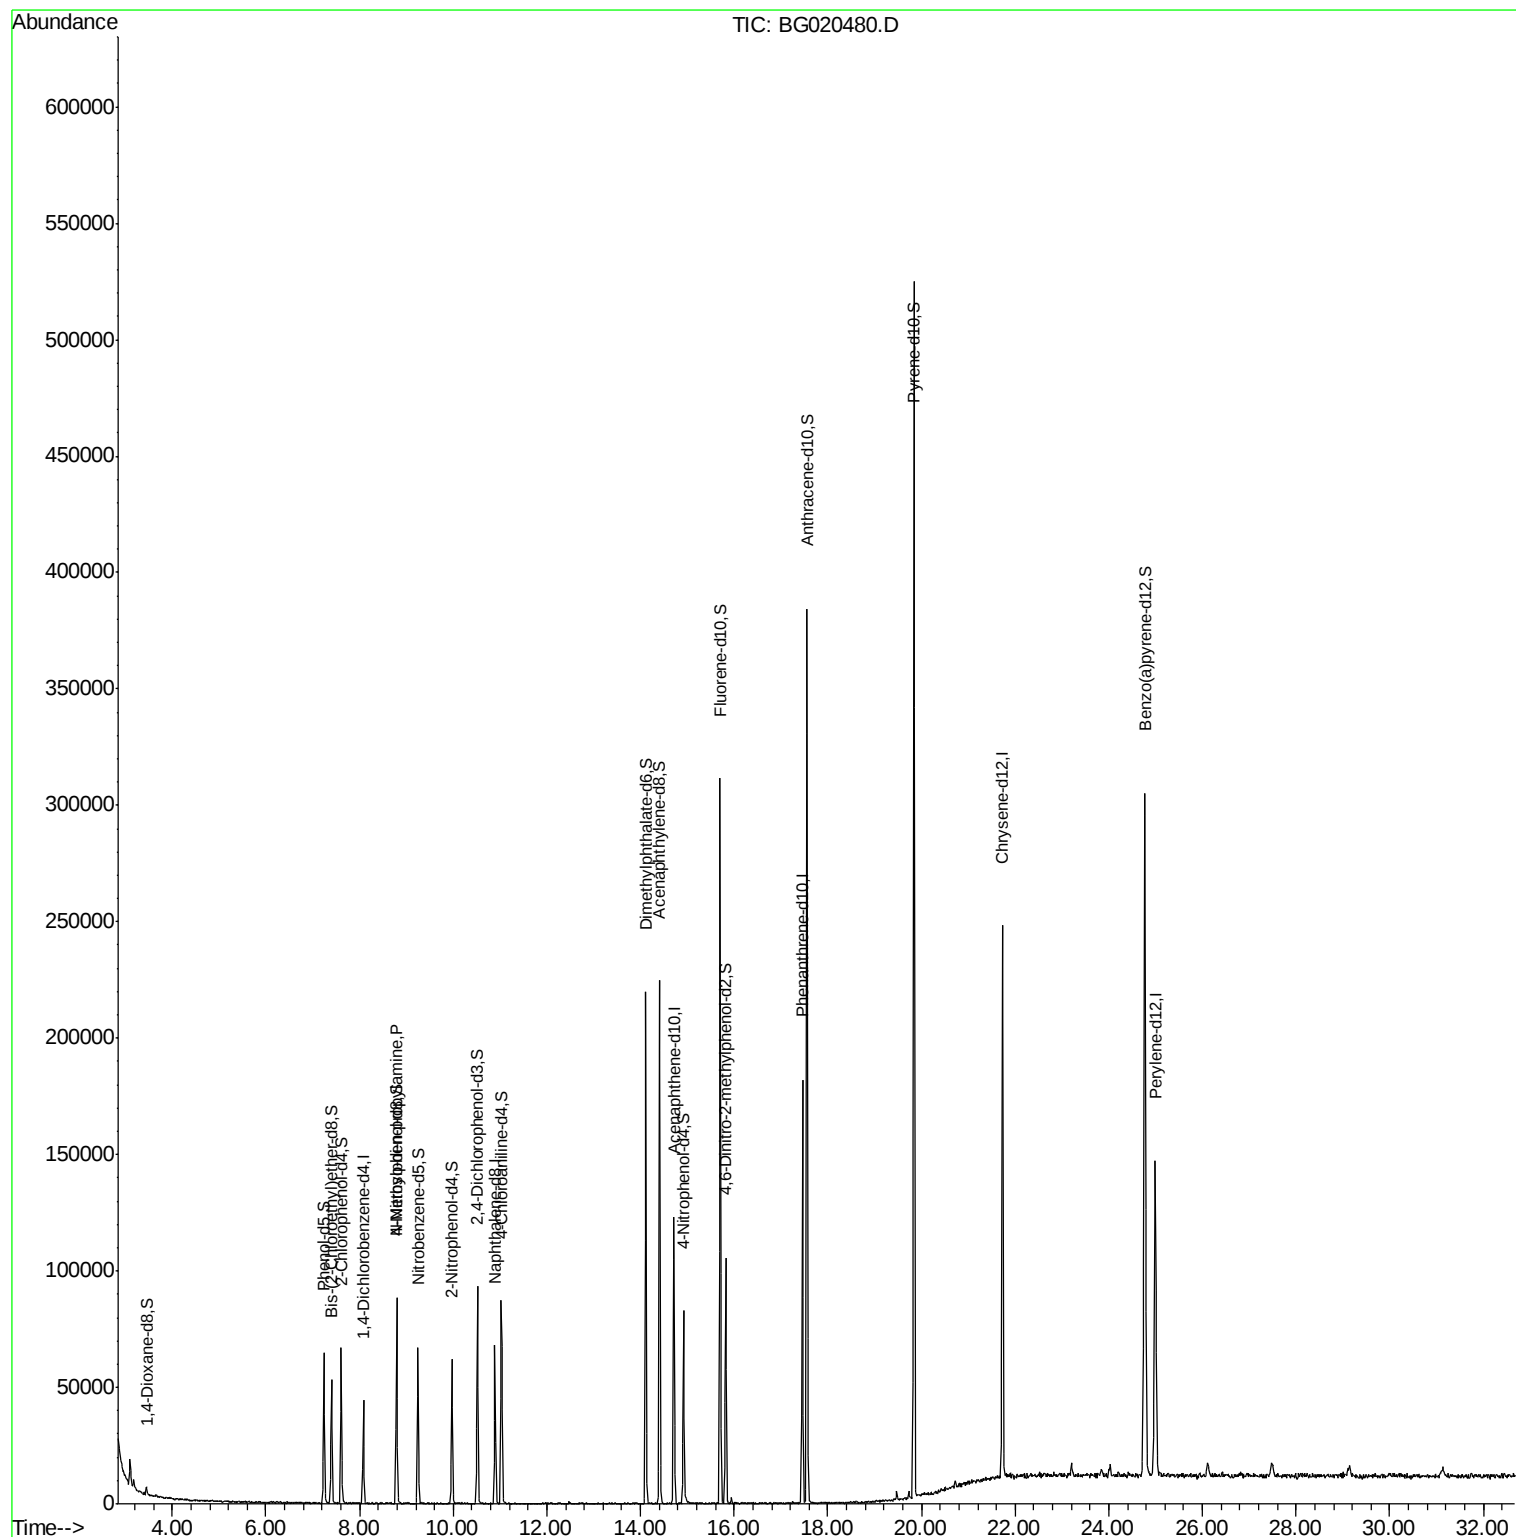

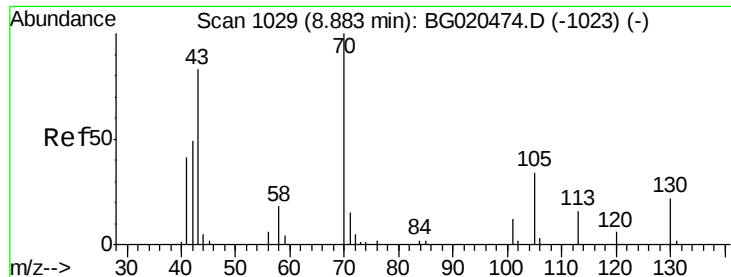

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.05 ng/ul
 RT: 8.78 min Scan# 1012
 Delta R.T. -0.10 min
 Lab File: BG020480.D
 Acq: 24 Dec 2015 19:48

Instrument :
 BNA_G
 ClientSampleId :
 SBLK62

Tgt Ion:	70	Resp:	784
Ion	Ratio	Lower	Upper
70	100		
42	322.9	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

