

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020484.D
 Acq On : 24 Dec 2015 22:27
 Operator : UM/SJ
 Sample : G4955BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK82

Quant Time: Dec 25 02:23:57 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 02:19:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	14071	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	62454	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	46380	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	126154	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	165448	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	156522	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	1507	5.91	ng/uL	0.00
5) Phenol-d5	7.24	99	38356	33.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	23794	35.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	30774	35.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	34226	36.03	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	17052	34.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	20386	36.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	36132	33.54	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	35113	28.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	145450	38.05	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	159388	35.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	21078	33.07	ng/ul	0.00
58) Fluorene-d10	15.70	176	126409	36.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	19732	23.60	ng/ul	0.00
71) Anthracene-d10	17.56	188	226330	38.30	ng/ul	0.00
79) Pyrene-d10	19.84	212	282519	39.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	324111	40.96	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.78	70	824	1.07 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020484.D
Acq On : 24 Dec 2015 22:27
Operator : UM/SJ
Sample : G4955BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK82

Quant Time: Dec 25 02:23:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 02:19:33 2015
Response via : Initial Calibration

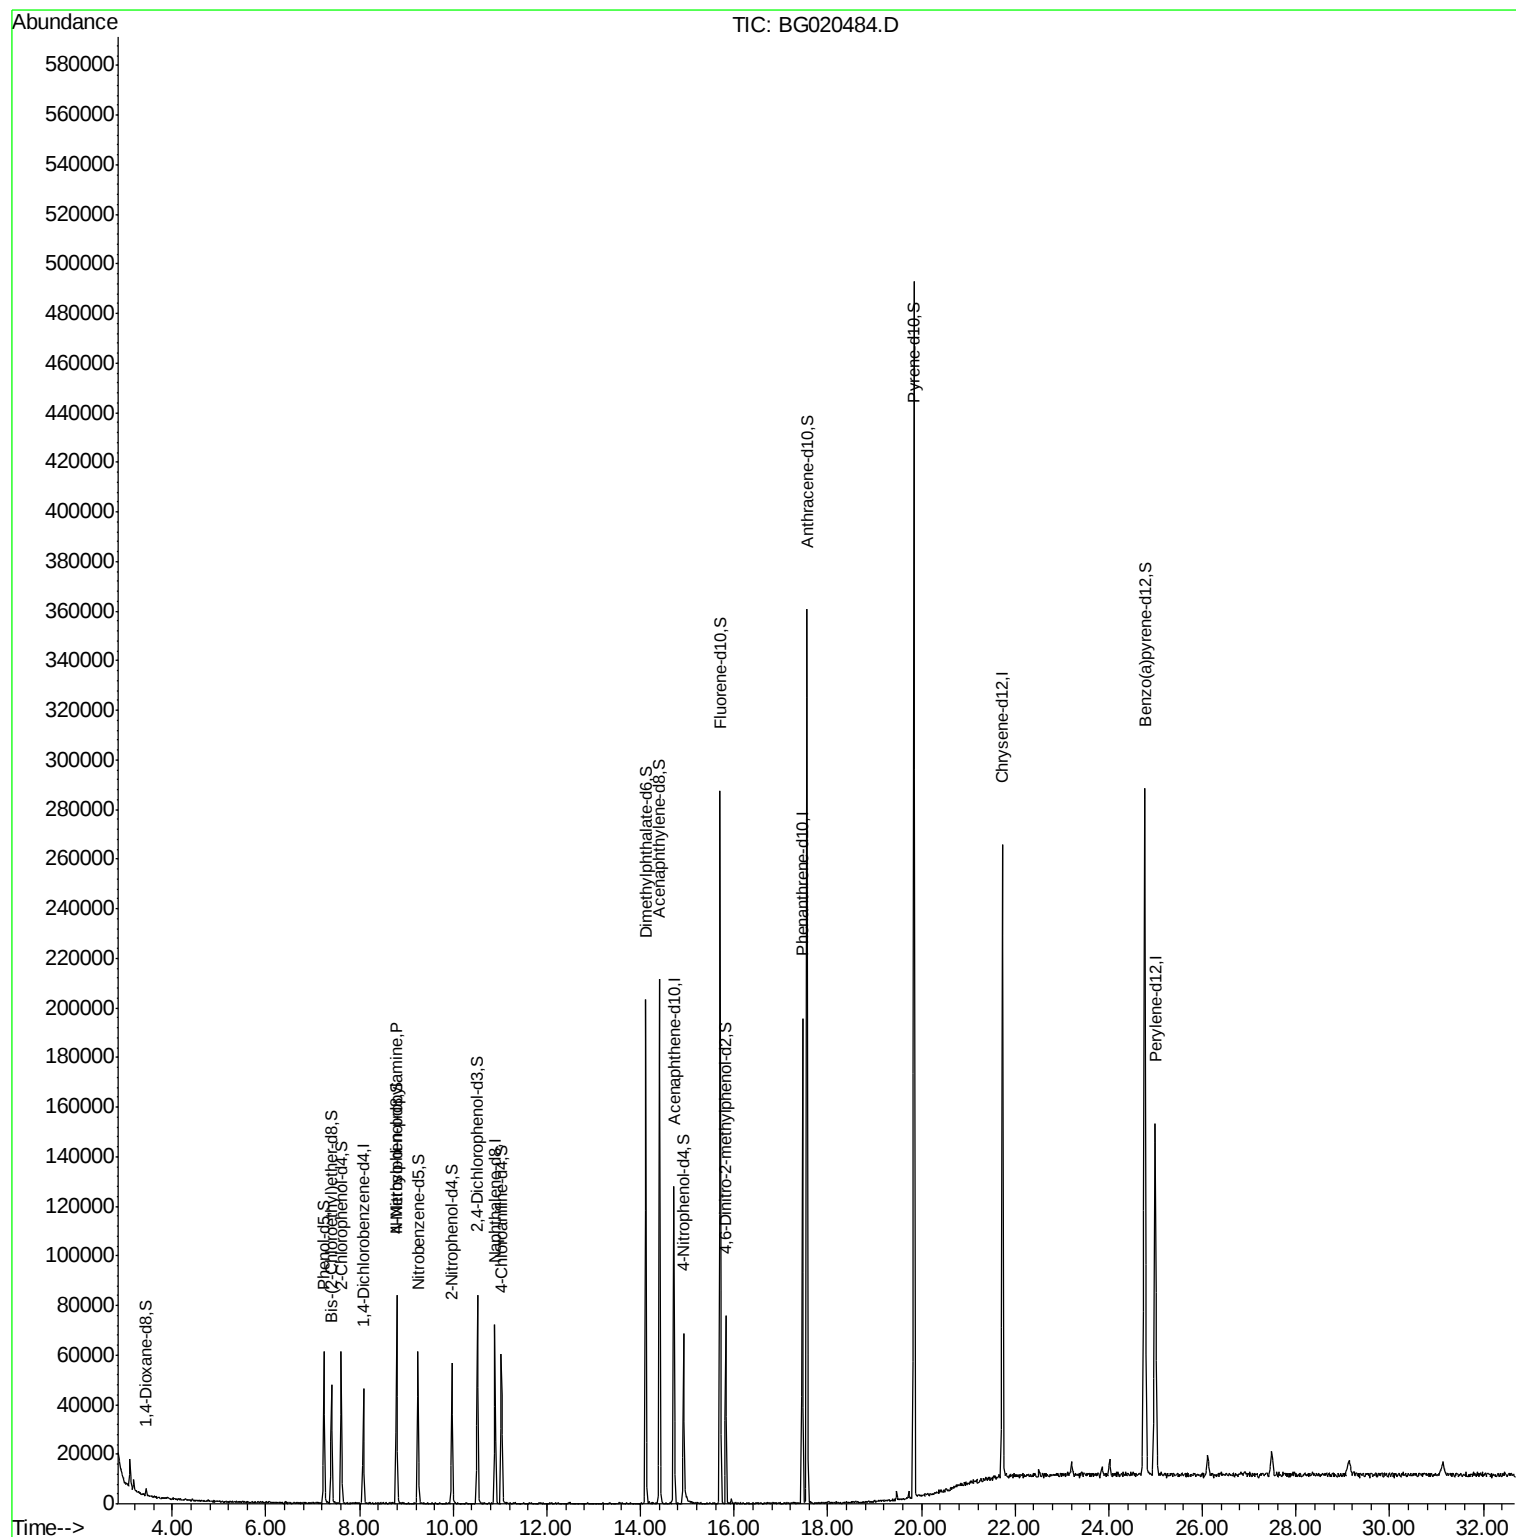

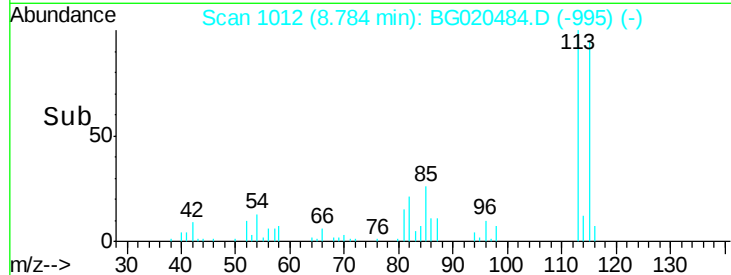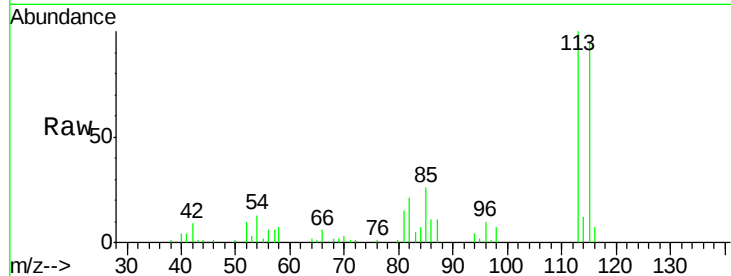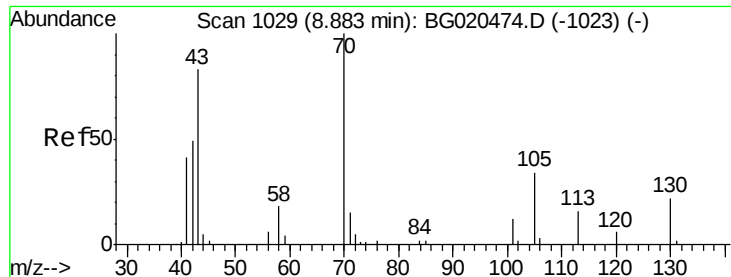

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.07 ng/ul
 RT: 8.78 min Scan# 1012
 Delta R.T. -0.10 min
 Lab File: BG020484.D
 Acq: 24 Dec 2015 22:27

Instrument :
 BNA_G
 ClientSampleId :
 SBLK82

Tgt Ion:	70	Resp:	824
Ion	Ratio	Lower	Upper
70	100		
42	300.5	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

