

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020488.D
 Acq On : 25 Dec 2015 1:05
 Operator : UM/SJ
 Sample : PB87436TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB09

Quant Time: Dec 25 03:31:06 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 03:27:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	16398	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	67742	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	49161	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	133029	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	169314	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	165263	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	2169	7.30	ng/uL	0.00
5) Phenol-d5	7.24	99	48553	36.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	29433	37.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	38974	38.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	41652	37.62	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	21243	40.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	24154	40.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	43558	37.28	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	58424	43.76	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	166042	40.98	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	186793	39.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	23416	34.66	ng/ul	0.00
58) Fluorene-d10	15.70	176	144246	39.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	21656	24.56	ng/ul	0.00
71) Anthracene-d10	17.56	188	249911	40.11	ng/ul	0.00
79) Pyrene-d10	19.84	212	308416	42.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	344802	41.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	955	1.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020488.D
Acq On : 25 Dec 2015 1:05
Operator : UM/SJ
Sample : PB87436TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB09

Quant Time: Dec 25 03:31:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 03:27:34 2015
Response via : Initial Calibration

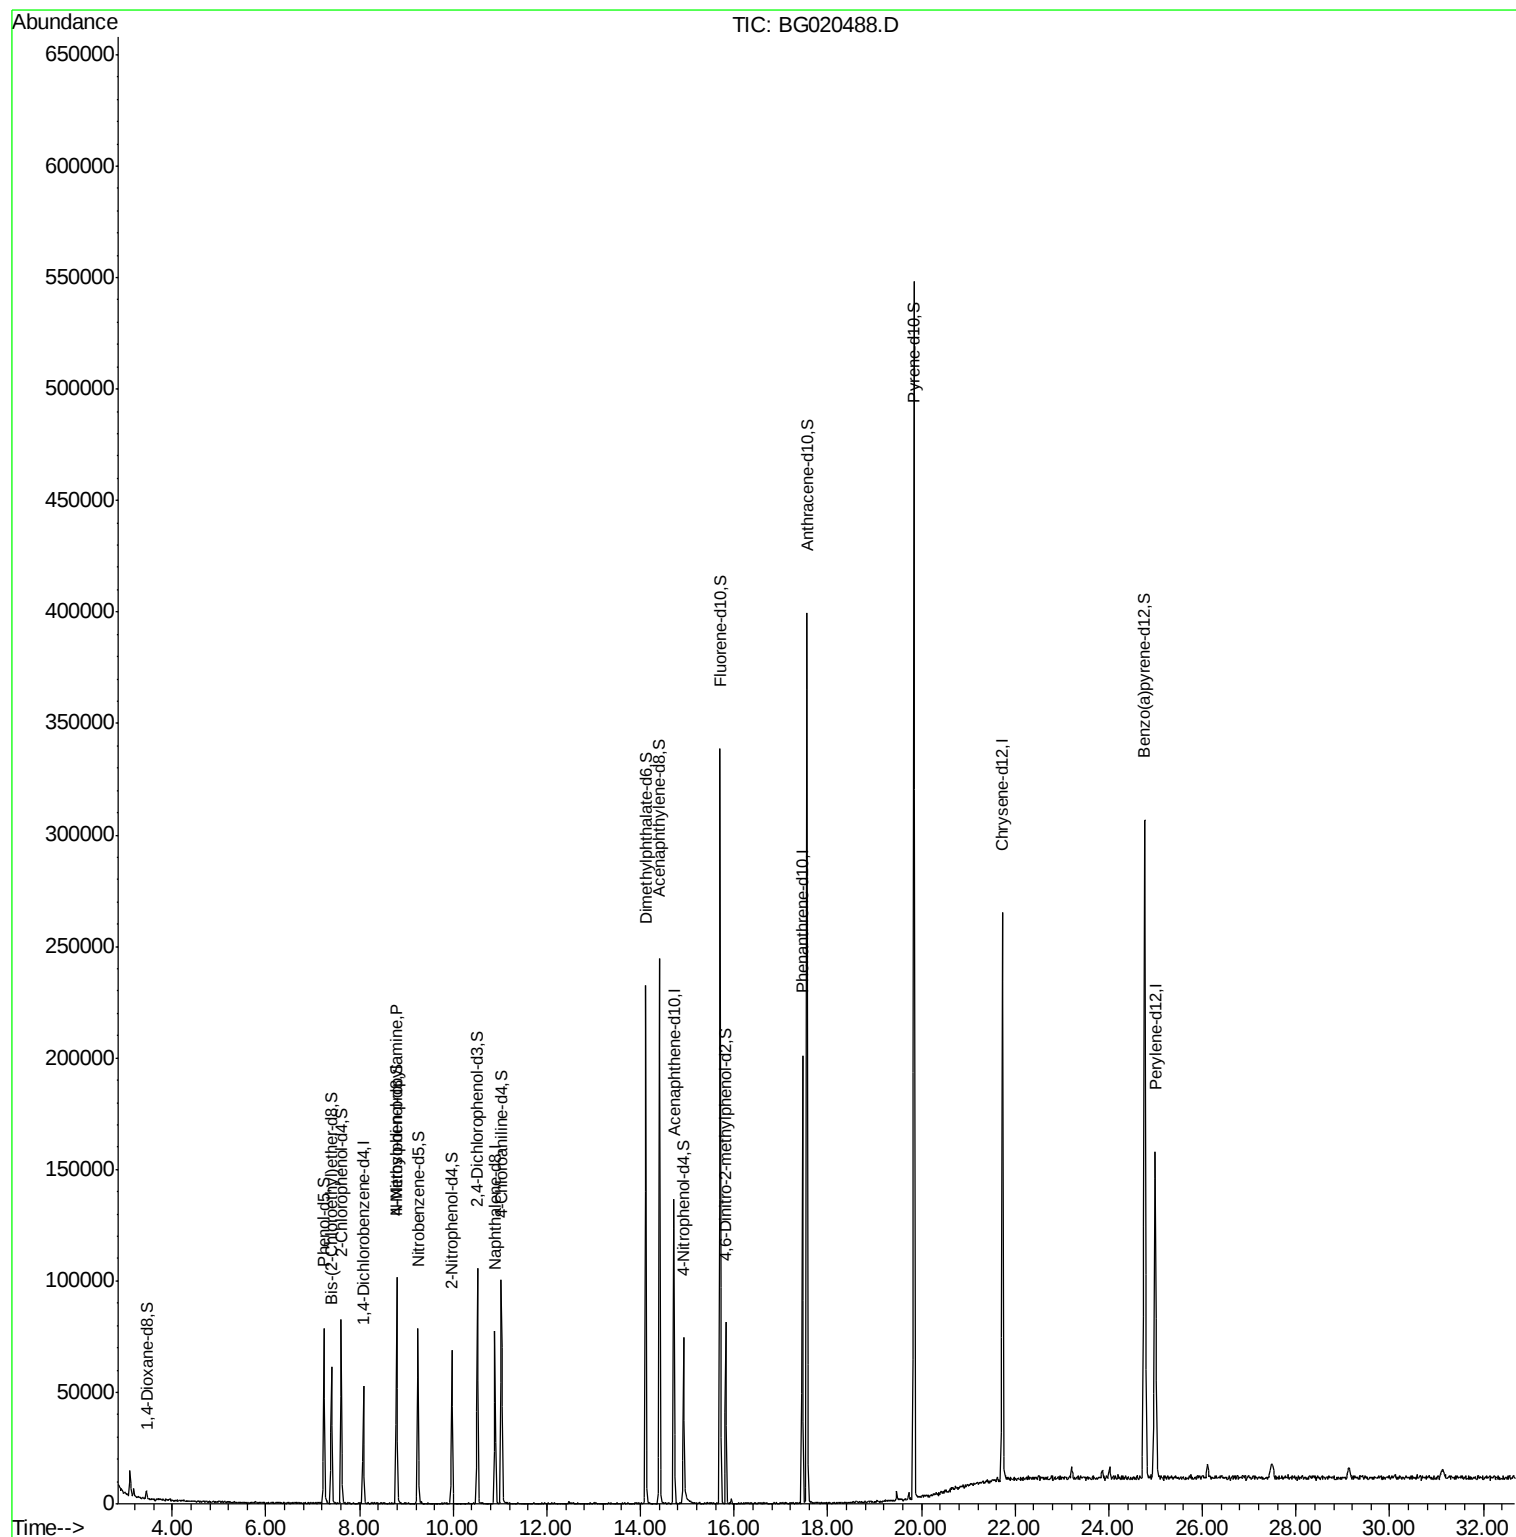

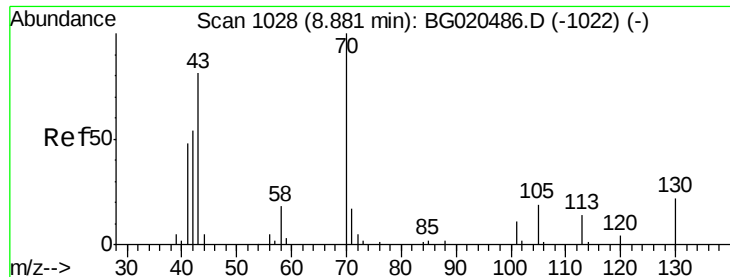

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.06 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.09 min
 Lab File: BG020488.D
 Acq: 25 Dec 2015 1:05

Instrument :
 BNA_G
 ClientSampleId :
 SLEB09

Tgt Ion:	70	Resp:	955
Ion	Ratio	Lower	Upper
70	100		
42	315.3	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

