

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020489.D
 Acq On : 25 Dec 2015 1:45
 Operator : UM/SJ
 Sample : PB87437BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK37

Quant Time: Dec 25 03:31:17 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 03:27:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	16867	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	73733	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	53722	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	144067	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	185998	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	177369	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	2472	8.08	ng/uL	0.00
5) Phenol-d5	7.24	99	50865	37.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	32854	40.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	41306	39.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	45232	39.72	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	22641	39.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	27105	41.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.51	165	49031	38.55	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	65716	45.23	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	181142	40.91	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	204967	39.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	23594	31.96	ng/ul	0.00
58) Fluorene-d10	15.70	176	160720	40.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	23368	24.47	ng/ul	0.00
71) Anthracene-d10	17.55	188	272176	40.33	ng/ul	0.00
79) Pyrene-d10	19.84	212	332068	41.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	369938	41.26	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	1047	1.14 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020489.D
Acq On : 25 Dec 2015 1:45
Operator : UM/SJ
Sample : PB87437BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK37

Quant Time: Dec 25 03:31:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 03:27:34 2015
Response via : Initial Calibration

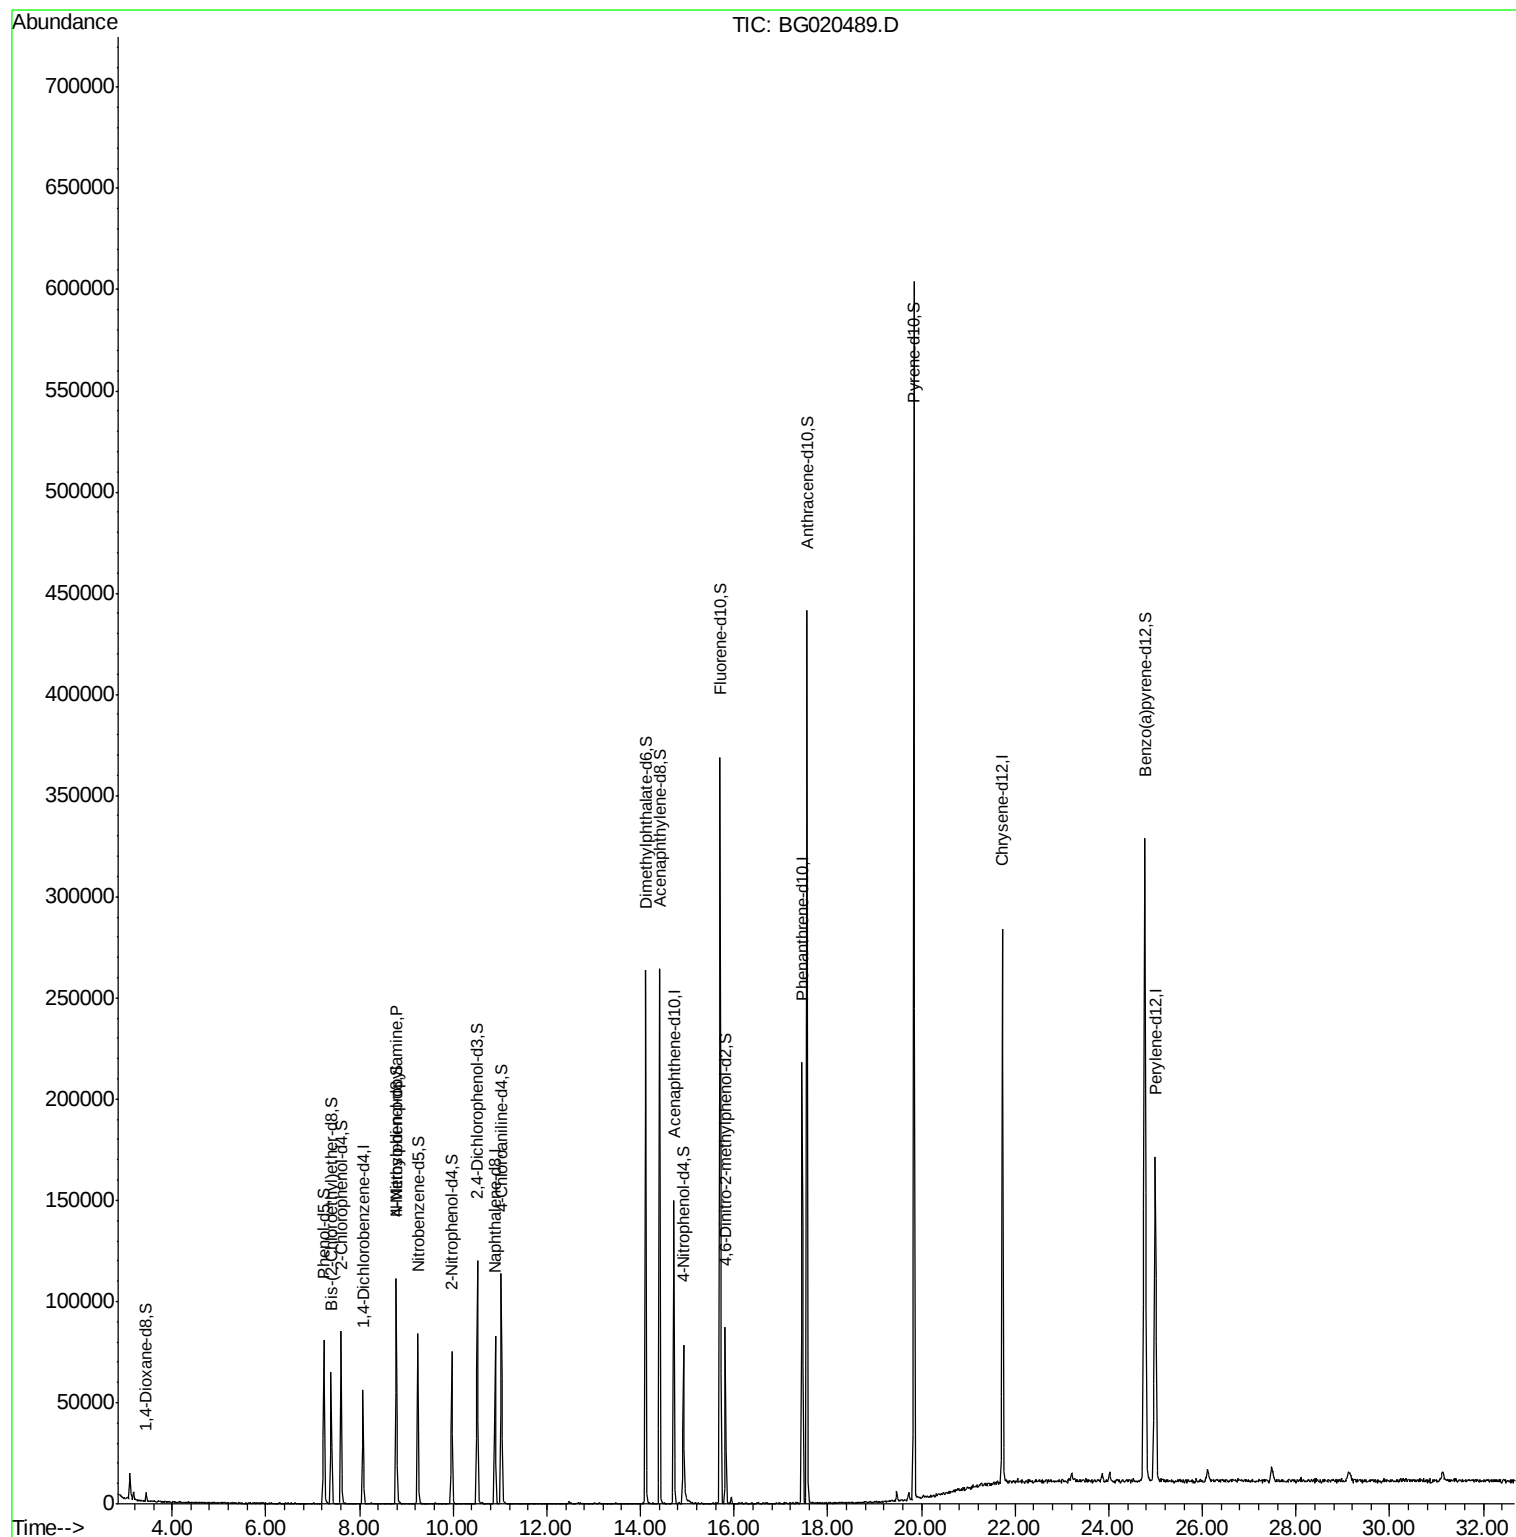

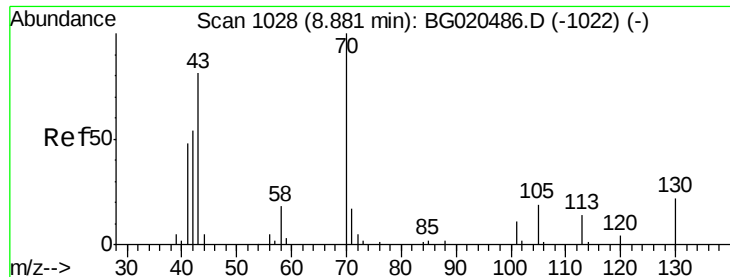

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.14 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.09 min
 Lab File: BG020489.D
 Acq: 25 Dec 2015 1:45

Instrument :
 BNA_G
 ClientSampleId :
 SBLK37

Tgt Ion:	70	Resp:	1047
Ion	Ratio	Lower	Upper
70	100		
42	283.4	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

