

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
 Data File : BG020490.D
 Acq On : 25 Dec 2015 2:25
 Operator : UM/SJ
 Sample : PB87437TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB11

Quant Time: Dec 25 03:31:29 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 03:27:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	15350	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	64518	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	46677	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	125213	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	164011	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	154909	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	2205	7.92	ng/uL	0.00
5) Phenol-d5	7.24	99	45240	36.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	28679	39.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	37519	39.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	39184	37.81	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	20640	40.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	23662	41.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	42749	38.42	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	57977	45.60	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	157587	40.96	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	176610	39.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	20913	32.61	ng/ul	0.00
58) Fluorene-d10	15.70	176	136683	39.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	20416	24.60	ng/ul	0.00
71) Anthracene-d10	17.56	188	239908	40.91	ng/ul	0.00
79) Pyrene-d10	19.84	212	298413	42.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	330891	42.25	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	1017	1.21 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122415\
Data File : BG020490.D
Acq On : 25 Dec 2015 2:25
Operator : UM/SJ
Sample : PB87437TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB11

Quant Time: Dec 25 03:31:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 03:27:34 2015
Response via : Initial Calibration

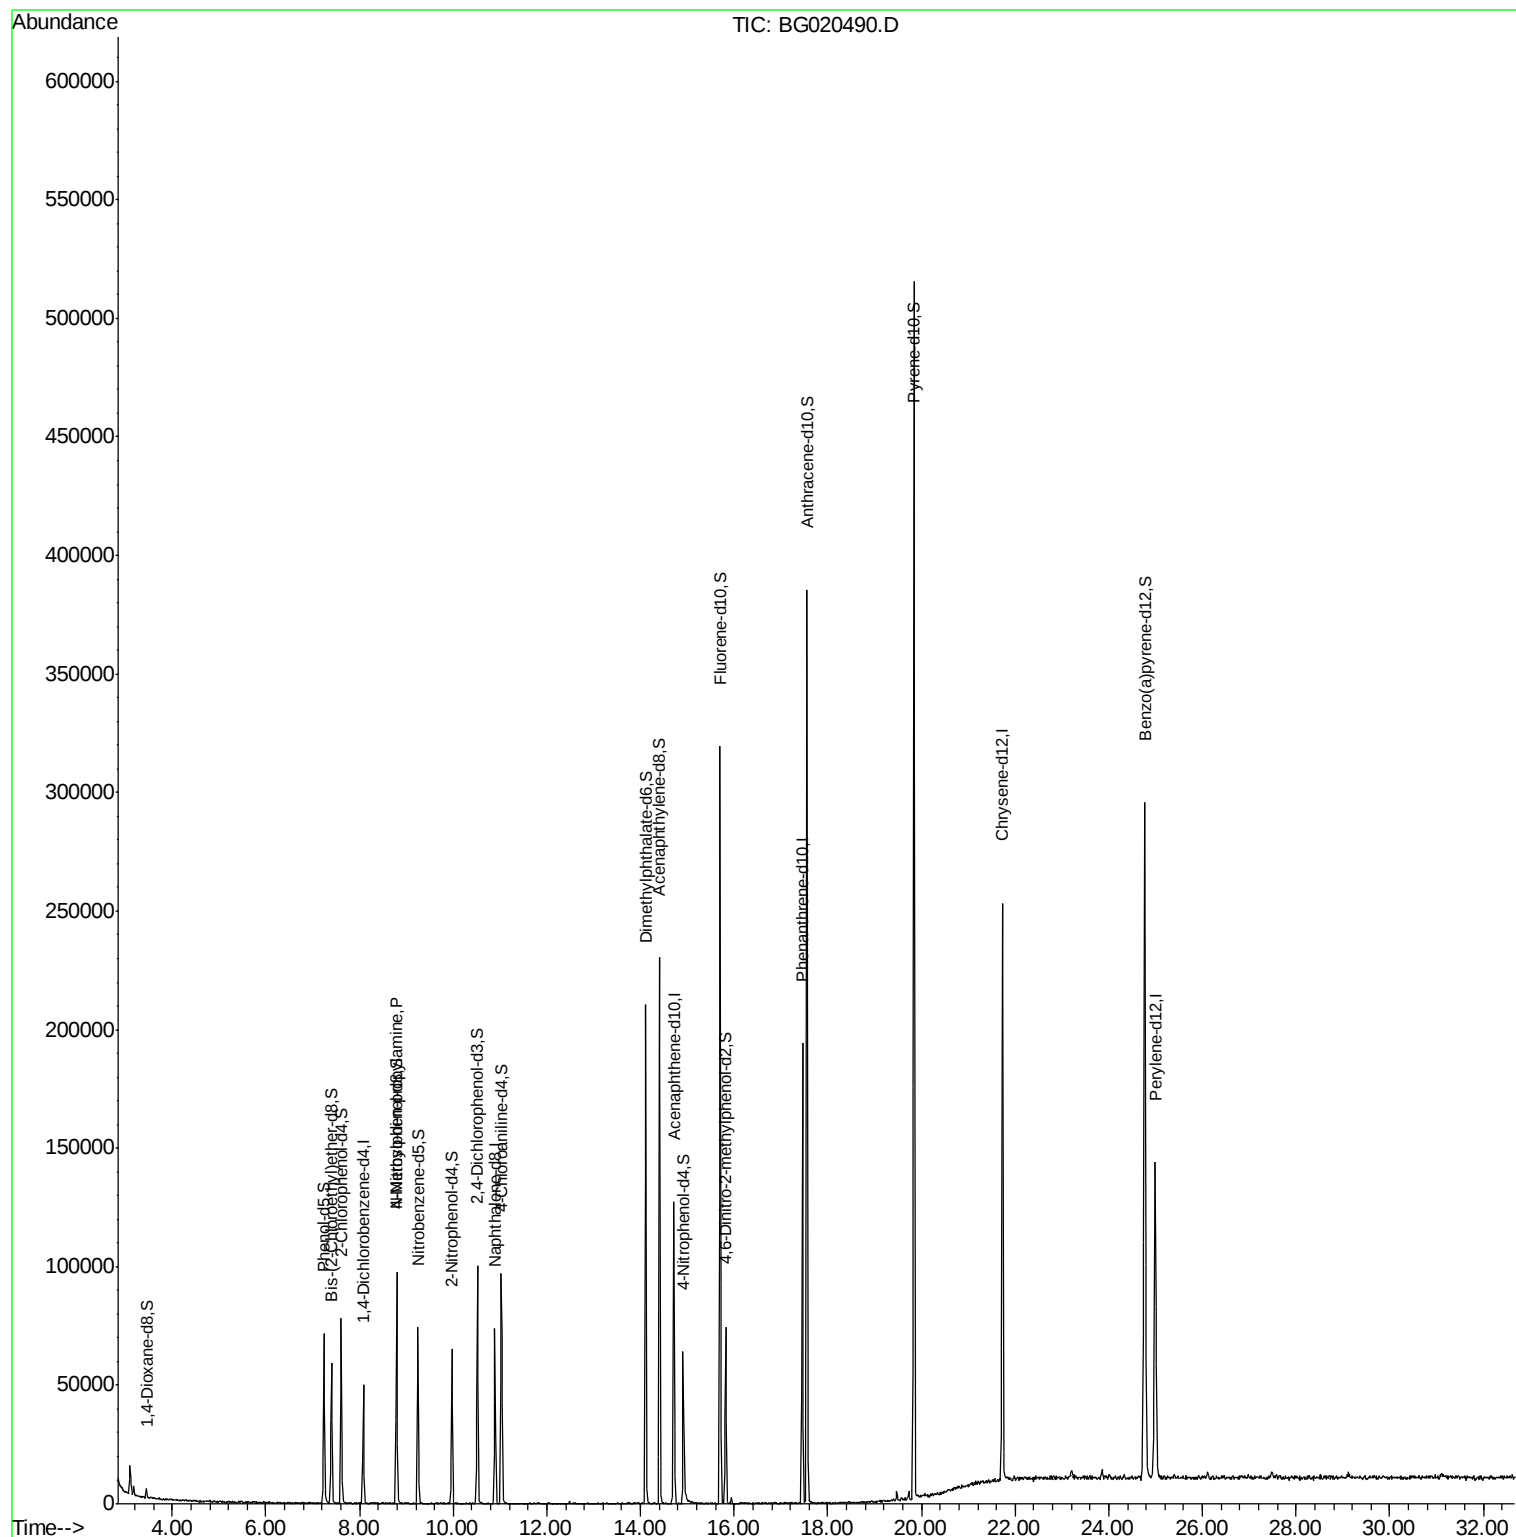

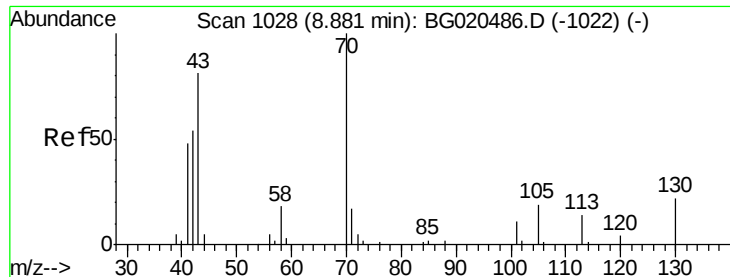

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.21 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.09 min
 Lab File: BG020490.D
 Acq: 25 Dec 2015 2:25

Instrument :
 BNA_G
 ClientSampleId :
 SLEB11

Tgt Ion: 70 Resp: 1017
 Ion Ratio Lower Upper
 70 100
 42 254.9 44.3 66.5#
 101 0.0 7.6 11.4#
 130 0.0 17.0 25.4#

