

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122415\
 Data File : BG020492.D
 Acq On : 25 Dec 2015 3:44
 Operator : UM/SJ
 Sample : PB87438TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB12

Quant Time: Dec 25 07:50:31 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 25 03:27:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	15466	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	65927	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	48043	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	241754	20.00	ng/ul	0.10
78) Chrysene-d12	21.73	240	163367	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	154854	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	2108	7.52	ng/uL	0.00
5) Phenol-d5	7.24	99	46735	37.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	29314	39.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	38315	40.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	40800	39.07	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	20530	39.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	23943	40.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	42822	37.66	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	58869	45.31	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	162731	41.09	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	182630	39.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	18902	28.63	ng/ul	0.00
58) Fluorene-d10	15.70	176	141462	39.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.87	200	146	0.09	ng/ul	0.05
71) Anthracene-d10	17.55	188	241624	21.34	ng/ul	0.00
79) Pyrene-d10	19.83	212	297953	42.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	329812	42.13	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.79	70	975	1.15	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122415\
Data File : BG020492.D
Acq On : 25 Dec 2015 3:44
Operator : UM/SJ
Sample : PB87438TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB12

Quant Time: Dec 25 07:50:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 25 03:27:34 2015
Response via : Initial Calibration

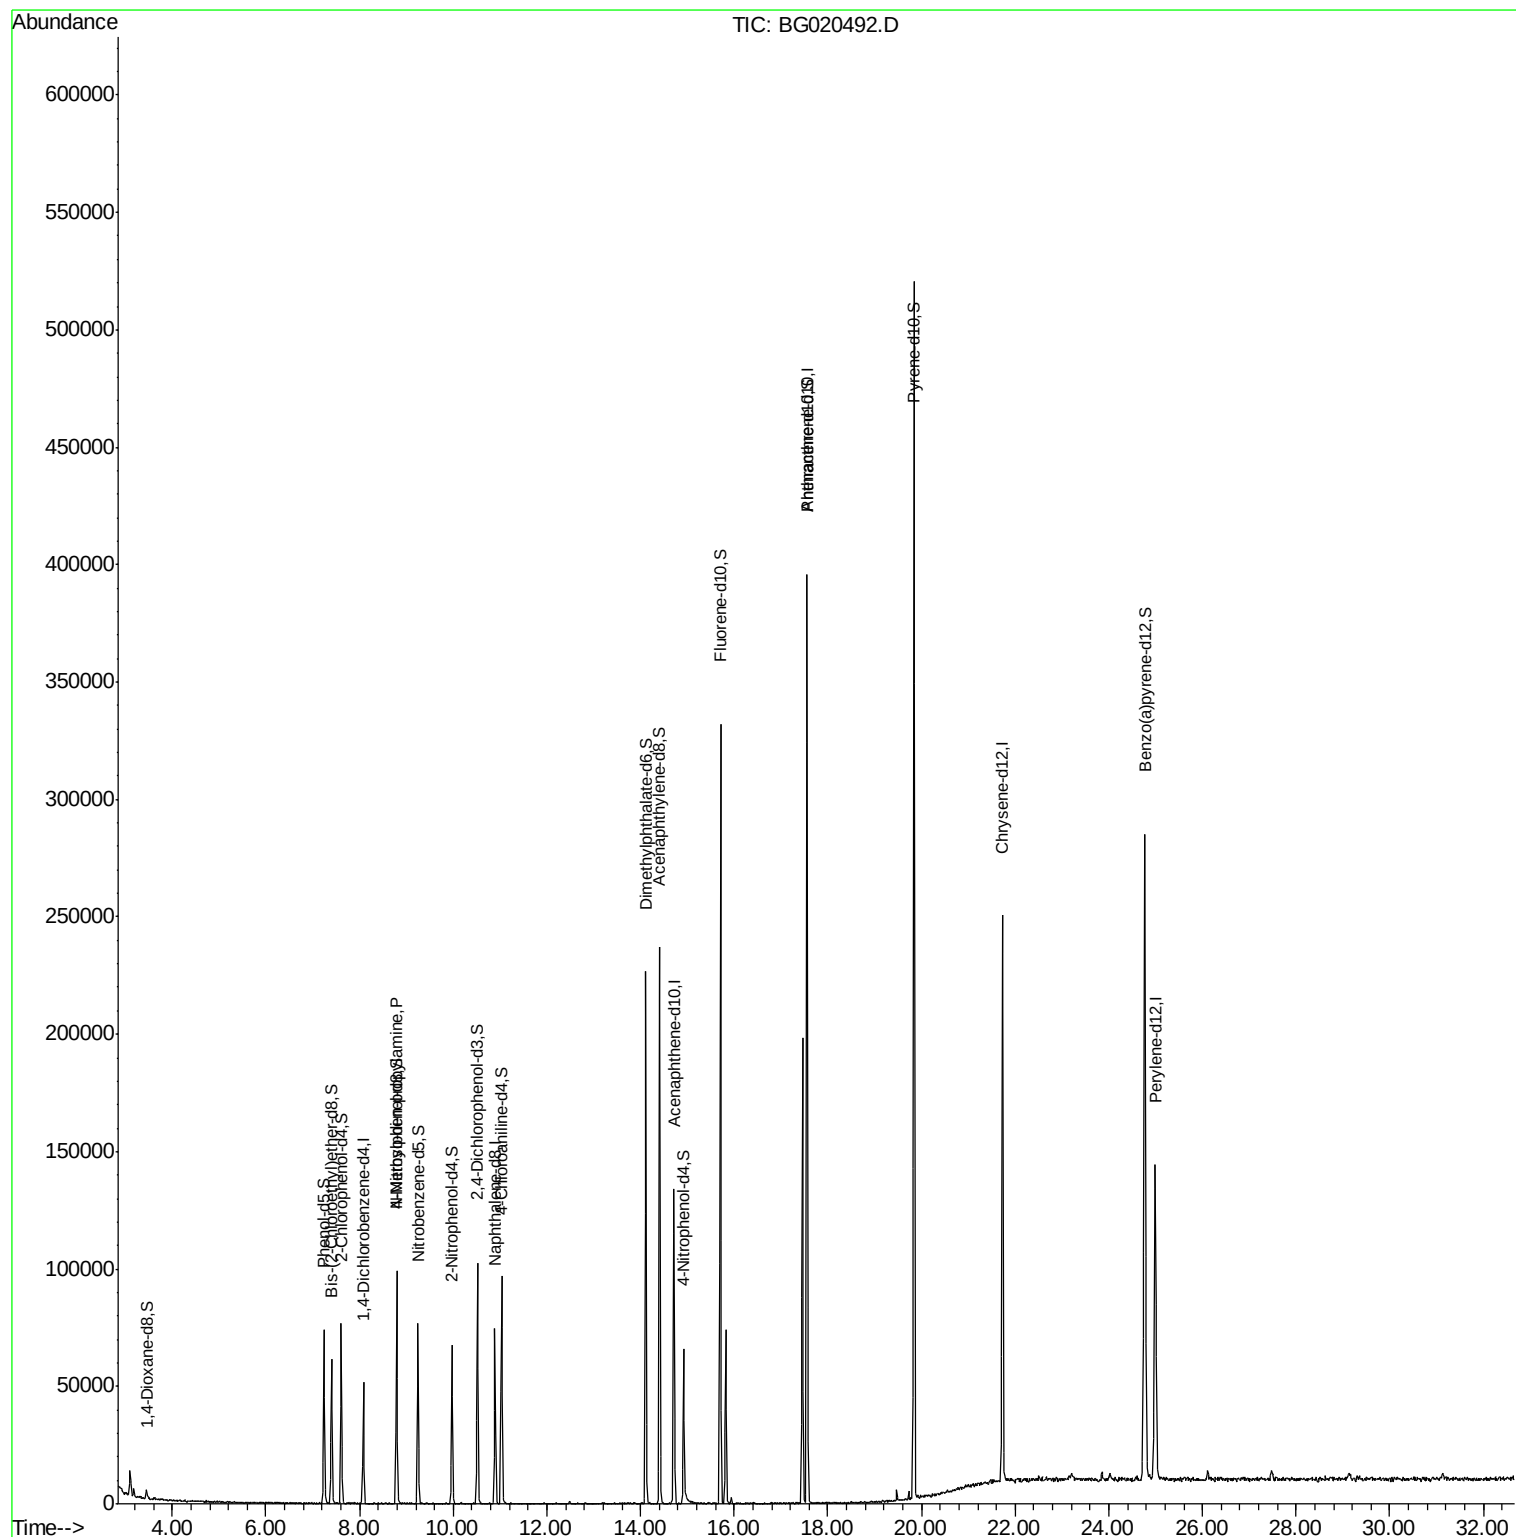

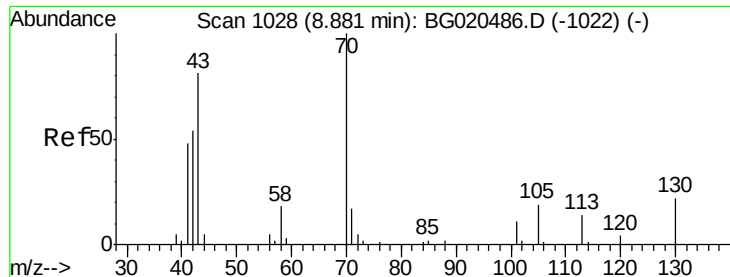

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.15 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.09 min
 Lab File: BG020492.D
 Acq: 25 Dec 2015 3:44

Instrument :
 BNA_G
 ClientSampleId :
 SLEB12

Tot Ion:	70	Resp:	975
Ion	Ratio	Lower	Upper
70	100		
42	315.5	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

