

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122515\
 Data File : BG020526.D
 Acq On : 26 Dec 2015 5:38
 Operator : UM/SJ
 Sample : G4802-06
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9D81

Quant Time: Dec 28 00:27:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 28 00:23:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	15099	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	65392	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	48474	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	132084	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	172689	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	167100	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	1796	6.56	ng/uL	0.00
5) Phenol-d5	7.23	99	40666	33.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	26552	36.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	33256	35.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.78	113	34065	33.42	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	17842	34.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	20883	35.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.51	165	38229	33.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	48344	37.52	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	143839	36.00	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	163942	35.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	21080	31.65	ng/ul	0.00
58) Fluorene-d10	15.70	176	132907	36.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	23274	26.59	ng/ul	0.00
71) Anthracene-d10	17.55	188	229638	37.12	ng/ul	0.00
79) Pyrene-d10	19.84	212	290116	38.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	320434	37.93	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.78	70	884	1.07	ng/ul#	1
45) Dimethylphthalate	14.15	163	48232	11.88	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122515\
Data File : BG020526.D
Acq On : 26 Dec 2015 5:38
Operator : UM/SJ
Sample : G4802-06
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9D81

Quant Time: Dec 28 00:27:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 28 00:23:46 2015
Response via : Initial Calibration




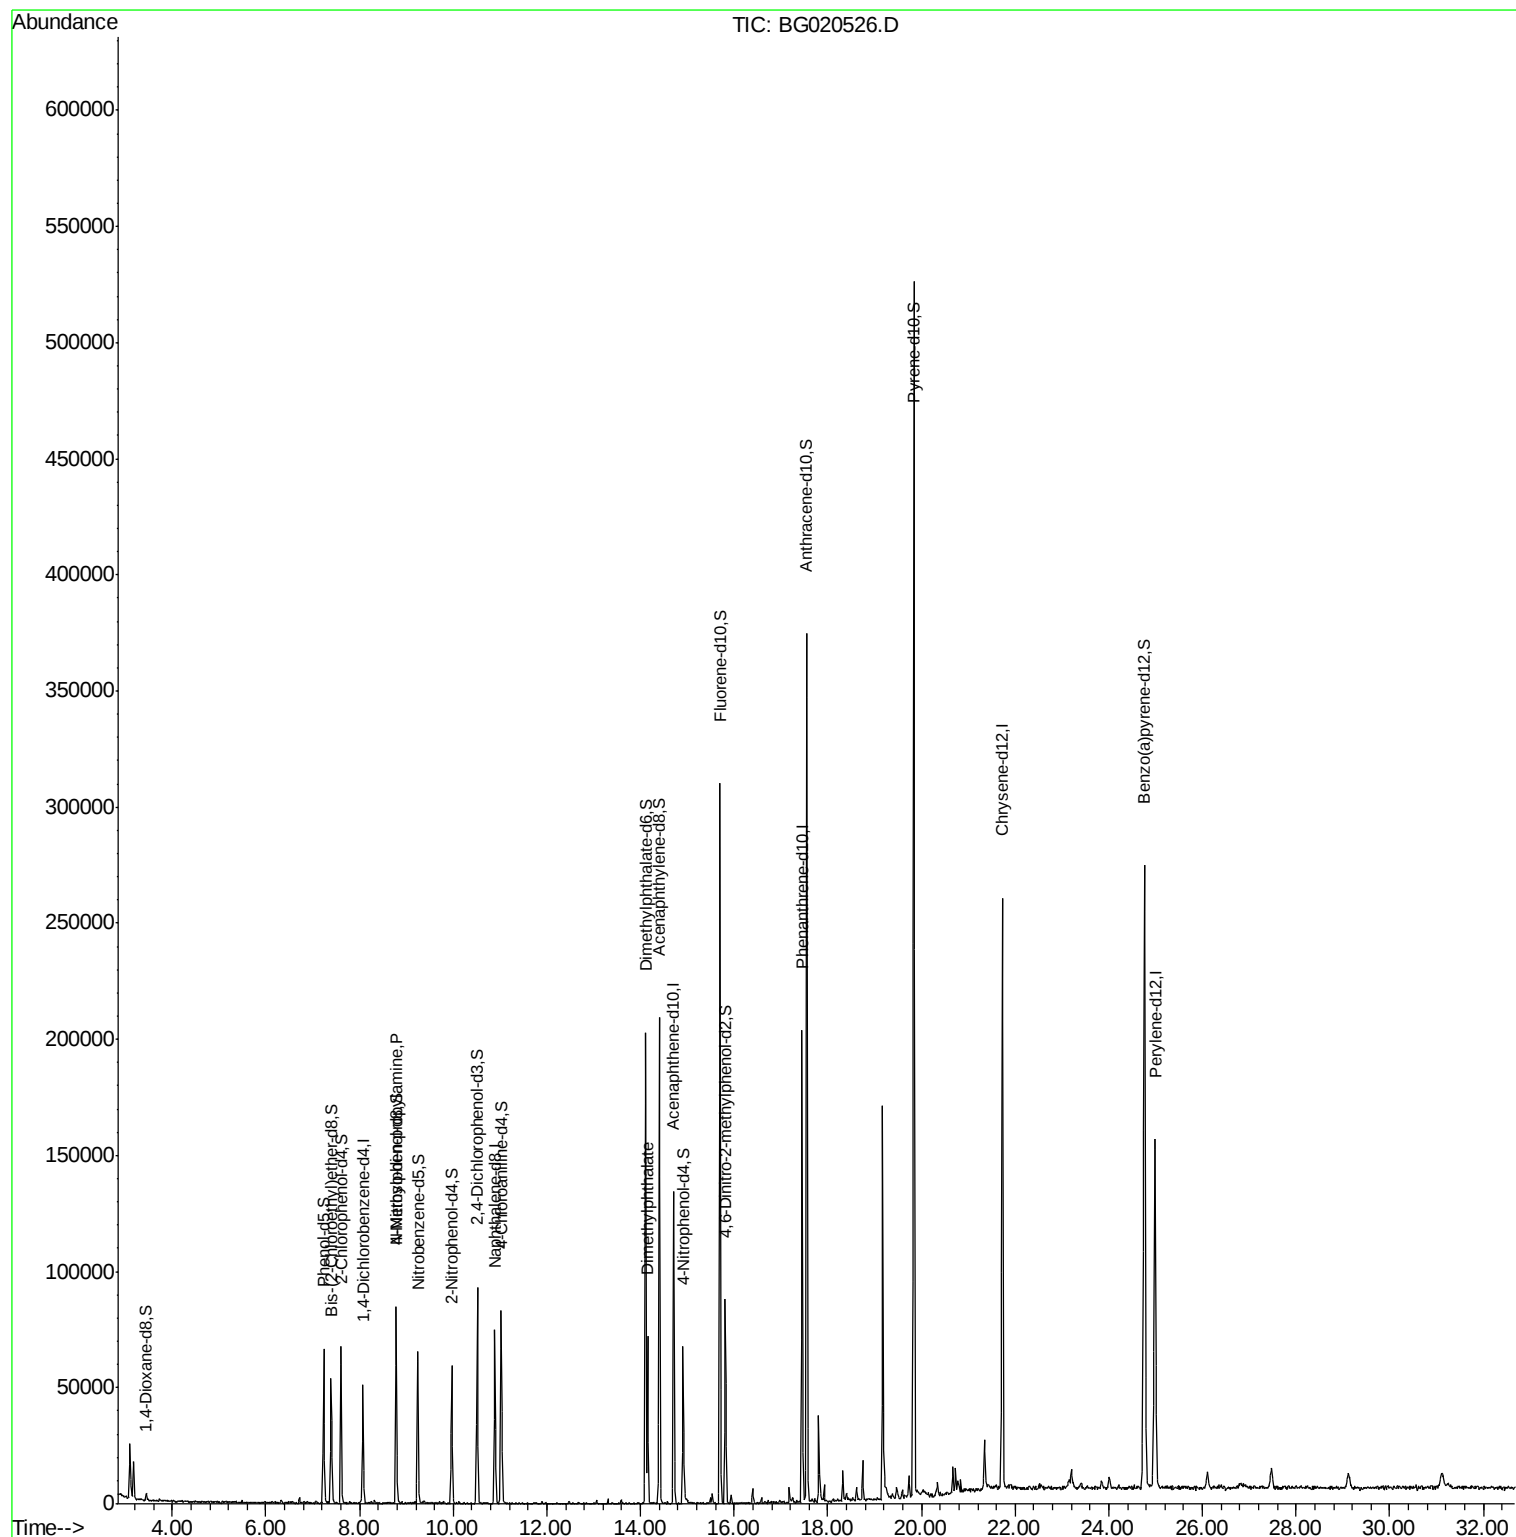


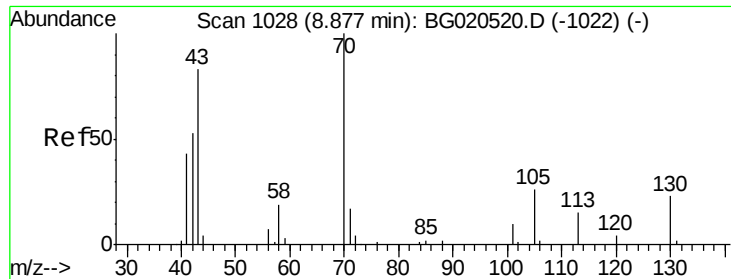

#15
N-Nitroso-di-n-propylamine
Concen: 1.07 ng/ul
RT: 8.78 min Scan# 1011
Delta R.T. -0.10 min
Lab File: BG020526.D
Acq: 26 Dec 2015 5:38

Instrument :
BNA_G
ClientSampleId :
G9D81

Tgt Ion: 70 Resp: 884
Ion Ratio Lower Upper
70 100
42 297.9 44.3 66.5#
101 0.0 7.6 11.4#
130 0.0 17.0 25.4#

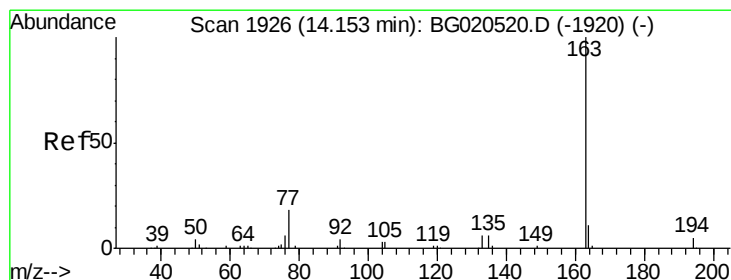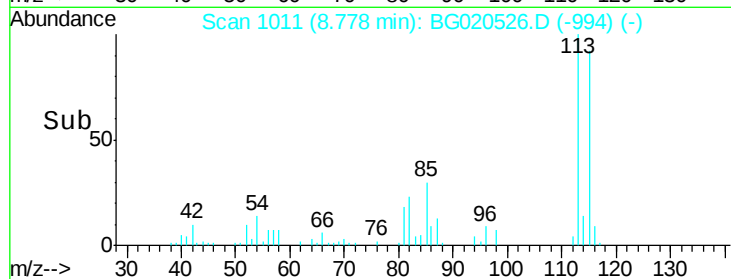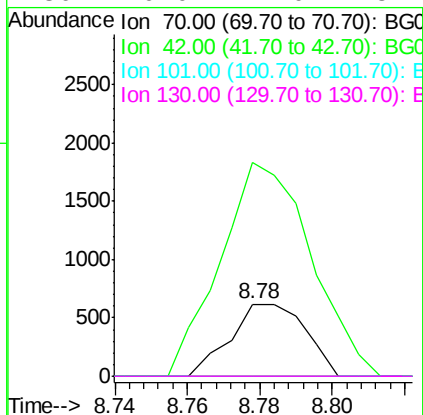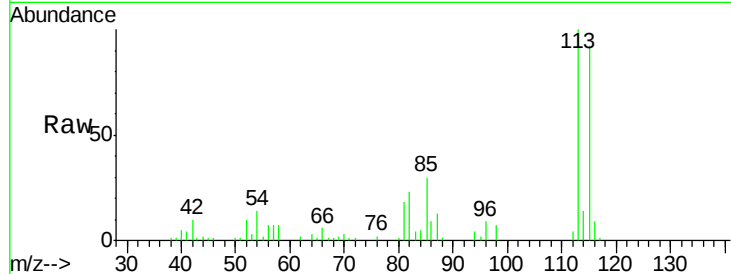

#45
Dimethylphthalate
Concen: 11.88 ng/ul
RT: 14.15 min Scan# 1926
Delta R.T. 0.00 min
Lab File: BG020526.D
Acq: 26 Dec 2015 5:38

Tgt Ion: 163 Resp: 48232
Ion Ratio Lower Upper
163 100
194 4.3 3.5 5.3
164 10.7 7.7 11.5

