

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122515\
 Data File : BG020524.D
 Acq On : 26 Dec 2015 4:20
 Operator : UM/SJ
 Sample : G4802-04
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9D79

Quant Time: Dec 28 00:45:34 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 28 00:23:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	15562	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	64733	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	49012	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	137710	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	179615	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	173061	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1780	6.31	ng/uL	0.00
5) Phenol-d5	7.23	99	42063	33.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	26519	35.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	33974	35.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.78	113	36339	34.59	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	18142	35.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	21580	37.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.51	165	39671	35.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	52032	40.79	ng/ul	0.00
44) Dimethylphthalate-d6	14.11	166	152727	37.81	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	172891	36.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	21319	31.65	ng/ul	0.00
58) Fluorene-d10	15.70	176	138430	37.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	26001	28.49	ng/ul	0.00
71) Anthracene-d10	17.55	188	241102	37.38	ng/ul	0.00
79) Pyrene-d10	19.84	212	305110	39.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	340295	38.90	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.15	163	82392	20.06	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122515\
Data File : BG020524.D
Acq On : 26 Dec 2015 4:20
Operator : UM/SJ
Sample : G4802-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9D79

Quant Time: Dec 28 00:45:34 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 28 00:23:46 2015
Response via : Initial Calibration

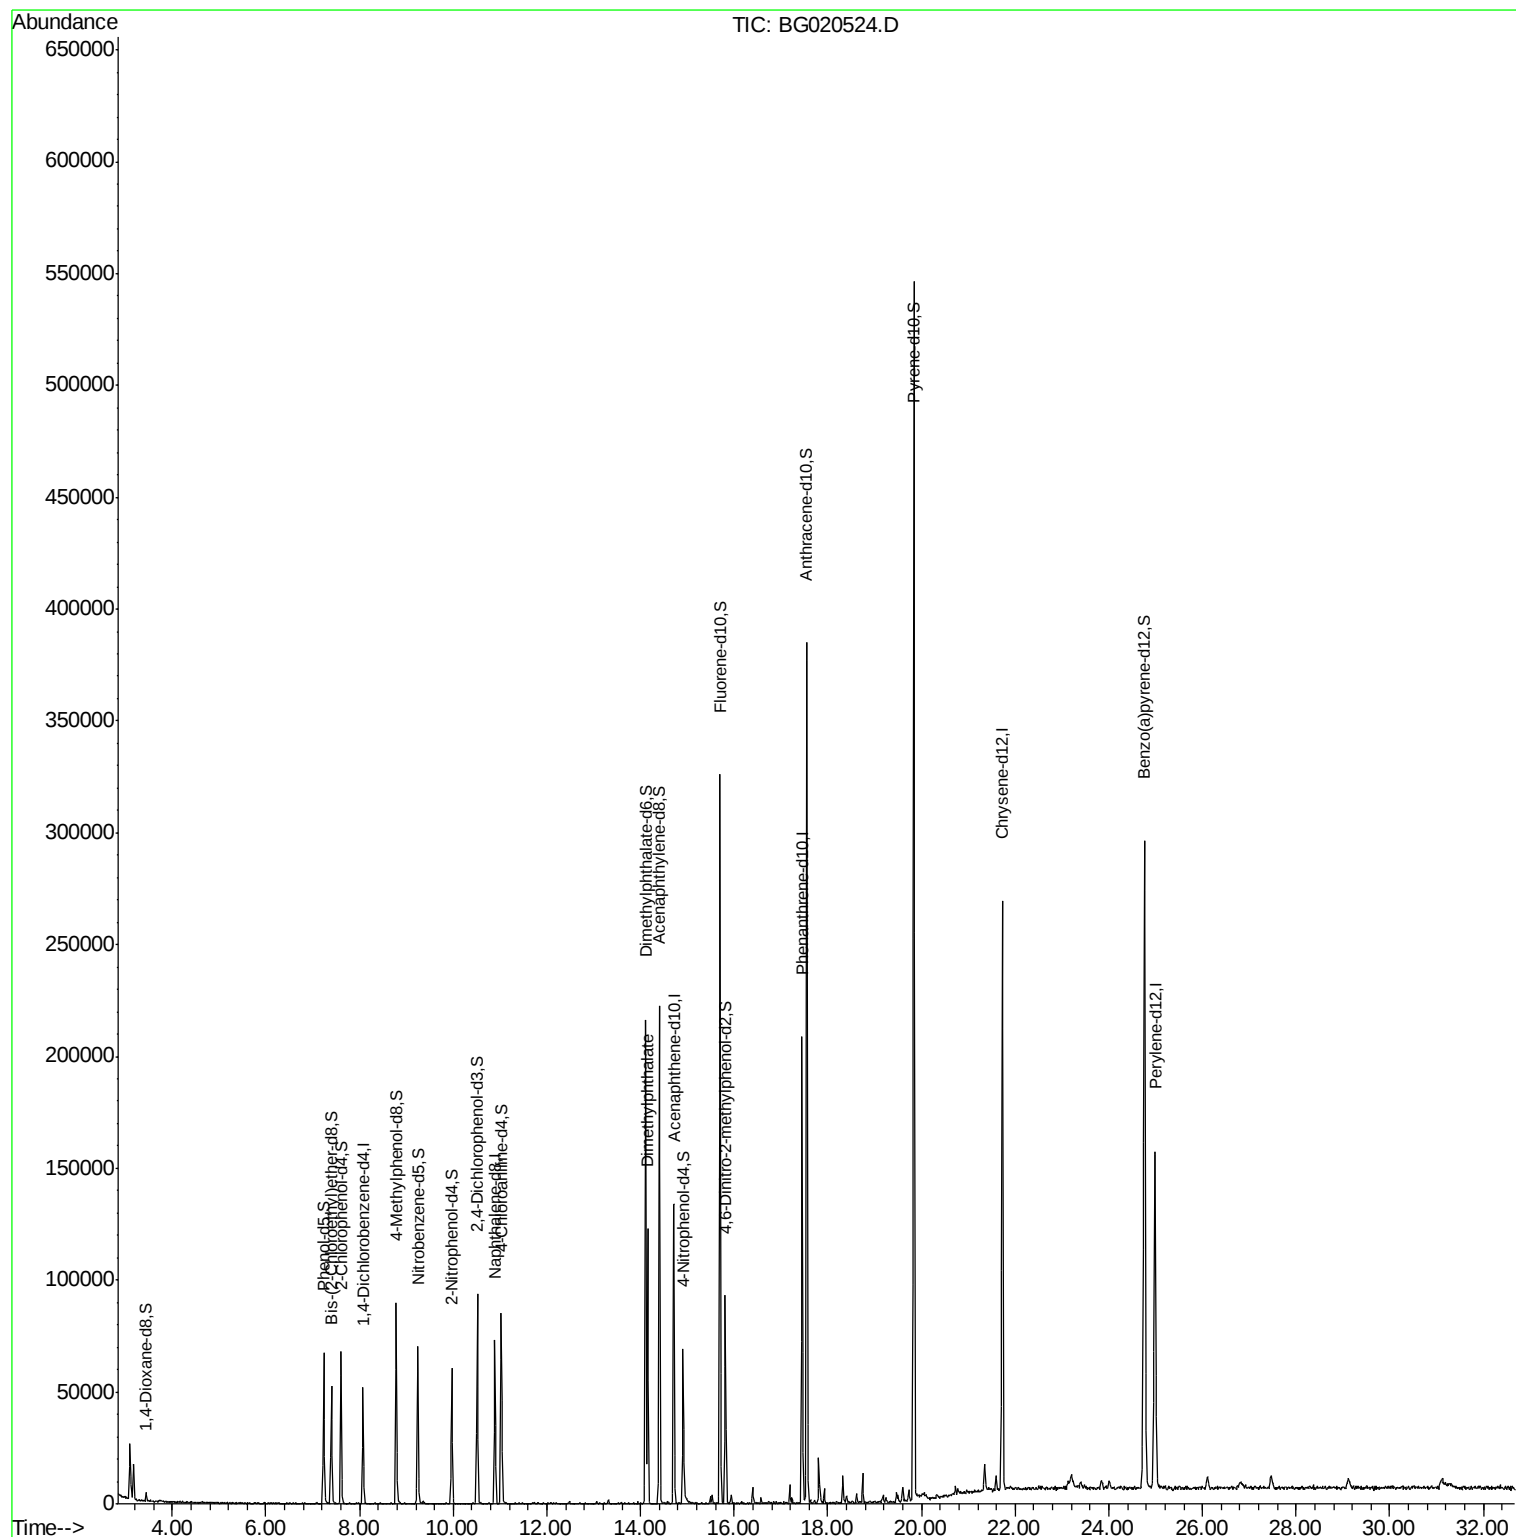

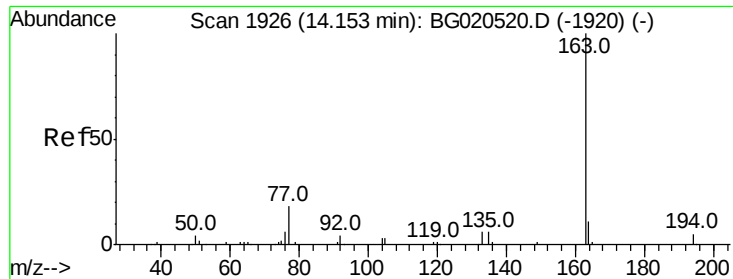

#45

Dimethylphthalate

Concen: 20.06 ng/ul

RT: 14.15 min Scan# 1926

Delta R.T. 0.00 min

Lab File: BG020524.D

Acq: 26 Dec 2015 4:20

Instrument :

BNA_G

ClientSampleId :

G9D79


Tot Ion:163 Resp: 82392

Ion Ratio Lower Upper

163 100

194 5.3 3.5 5.3#

164 9.6 7.7 11.5

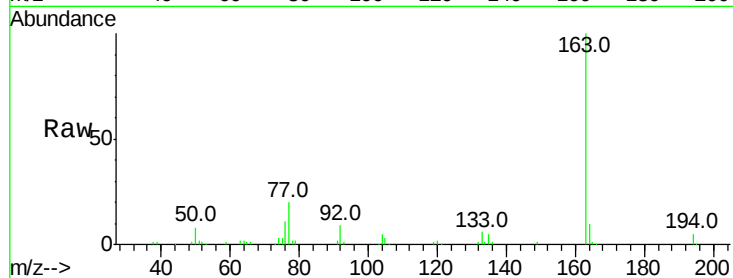

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

