

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122515\
 Data File : BG020506.D
 Acq On : 25 Dec 2015 15:49
 Operator : UM/SJ
 Sample : PB87434BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.102	40	45	54	rVB	12063	24881	3.25%	0.394%
2	3.173	54	57	66	rVB2	4395	7043	0.92%	0.111%
3	3.443	100	103	114	rVB3	3812	6052	0.79%	0.096%
4	4.976	361	364	367	rBV2	480	781	0.10%	0.012%
5	5.047	373	376	380	rBV	493	868	0.11%	0.014%
6	7.239	742	749	760	rBV	70097	123037	16.06%	1.948%
7	7.397	770	776	785	rBV	61093	97324	12.71%	1.541%
8	7.609	806	812	821	rBV	74420	126590	16.53%	2.004%
9	8.079	886	892	901	rBB	53332	89514	11.69%	1.417%
10	8.784	1005	1012	1022	rBV	93629	164953	21.54%	2.611%
11	9.242	1084	1090	1102	rBB	71442	133209	17.39%	2.109%
12	9.971	1208	1214	1224	rBV	65330	115555	15.09%	1.829%
13	10.511	1300	1306	1316	rBV	95961	174608	22.80%	2.764%
14	10.893	1364	1371	1378	rBV	76967	136616	17.84%	2.163%
15	11.028	1387	1394	1403	rBV	94808	174032	22.72%	2.755%
16	12.479	1637	1641	1645	rBB2	1035	1638	0.21%	0.026%
17	14.107	1912	1918	1928	rBV	219020	318097	41.53%	5.035%
18	14.407	1961	1969	1977	rBV	228850	360838	47.11%	5.712%
19	14.712	2014	2021	2028	rVB2	140806	222606	29.07%	3.524%
20	14.912	2049	2055	2071	rBV	67285	119957	15.66%	1.899%
21	15.024	2071	2074	2076	rVV	931	1199	0.16%	0.019%
22	15.699	2182	2189	2197	rBV	325772	486491	63.52%	7.701%
23	15.817	2203	2209	2217	rVB	93348	130396	17.03%	2.064%
24	15.940	2226	2230	2233	rBV2	2841	3480	0.45%	0.055%
25	17.250	2451	2453	2456	rVB2	804	830	0.11%	0.013%
26	17.456	2481	2488	2496	rBV	206570	307109	40.10%	4.862%
27	17.556	2498	2505	2517	rVB2	373617	579562	75.67%	9.175%
28	17.855	2552	2556	2558	rBV2	580	935	0.12%	0.015%
29	19.154	2775	2777	2780	rBV2	722	778	0.10%	0.012%
30	19.401	2817	2819	2822	rBV2	901	913	0.12%	0.014%
31	19.471	2827	2831	2835	rBV	3721	5569	0.73%	0.088%
32	19.606	2851	2854	2856	rBV2	1019	841	0.11%	0.013%
33	19.724	2869	2874	2879	rBV3	3163	4779	0.62%	0.076%
34	19.794	2882	2886	2887	rBV3	764	931	0.12%	0.015%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122515\
 Data File : BG020506.D
 Acq On : 25 Dec 2015 15:49
 Operator : UM/SJ
 Sample : PB87434BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
 Title : SVOA CALIBRATION

35	19.836	2887	2893	2904	rBV	542276	753687	98.41%	11.931%
36	20.053	2927	2930	2931	rVV3	1401	1073	0.14%	0.017%
37	20.088	2934	2936	2939	rVB4	846	939	0.12%	0.015%
38	20.129	2939	2943	2944	rBV3	964	1472	0.19%	0.023%
39	20.159	2946	2948	2952	rBV3	701	846	0.11%	0.013%
40	20.411	2990	2991	2995	rBV4	1146	1067	0.14%	0.017%
41	20.687	3034	3038	3041	rBV5	1183	1724	0.23%	0.027%
42	20.958	3082	3084	3085	rBV	1345	957	0.12%	0.015%
43	21.727	3208	3215	3225	rBV	266388	426550	55.69%	6.752%
44	21.857	3235	3237	3238	rBV2	1216	991	0.13%	0.016%
45	22.509	3346	3348	3353	rVB4	2245	1715	0.22%	0.027%
46	22.685	3376	3378	3383	rBV4	1379	1967	0.26%	0.031%
47	23.290	3479	3481	3482	rBV2	1525	1007	0.13%	0.016%
48	24.019	3600	3605	3610	rBV8	3576	7292	0.95%	0.115%
49	24.189	3632	3634	3636	rBV3	1360	1085	0.14%	0.017%
50	24.765	3721	3732	3746	rBV	276160	765881	100.00%	12.124%
51	24.988	3759	3770	3781	rBV	145587	404394	52.80%	6.402%
52	25.593	3871	3873	3874	rVB2	1837	1078	0.14%	0.017%
53	26.116	3954	3962	3969	rVB10	6031	14666	1.91%	0.232%
54	26.604	4043	4045	4047	rVB2	1683	800	0.10%	0.013%
55	27.462	4189	4191	4192	rBV2	2011	1655	0.22%	0.026%
56	30.100	4639	4640	4643	rVB3	2152	1200	0.16%	0.019%
57	30.129	4643	4645	4646	rBV2	1707	1165	0.15%	0.018%
58	30.194	4654	4656	4658	rBV2	1417	1042	0.14%	0.016%
59	30.452	4698	4700	4701	rBV2	1365	829	0.11%	0.013%


Sum of corrected areas: 6317094

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122515\
Data File : BG020506.D
Acq On : 25 Dec 2015 15:49
Operator : UM/SJ
Sample : PB87434BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK34

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

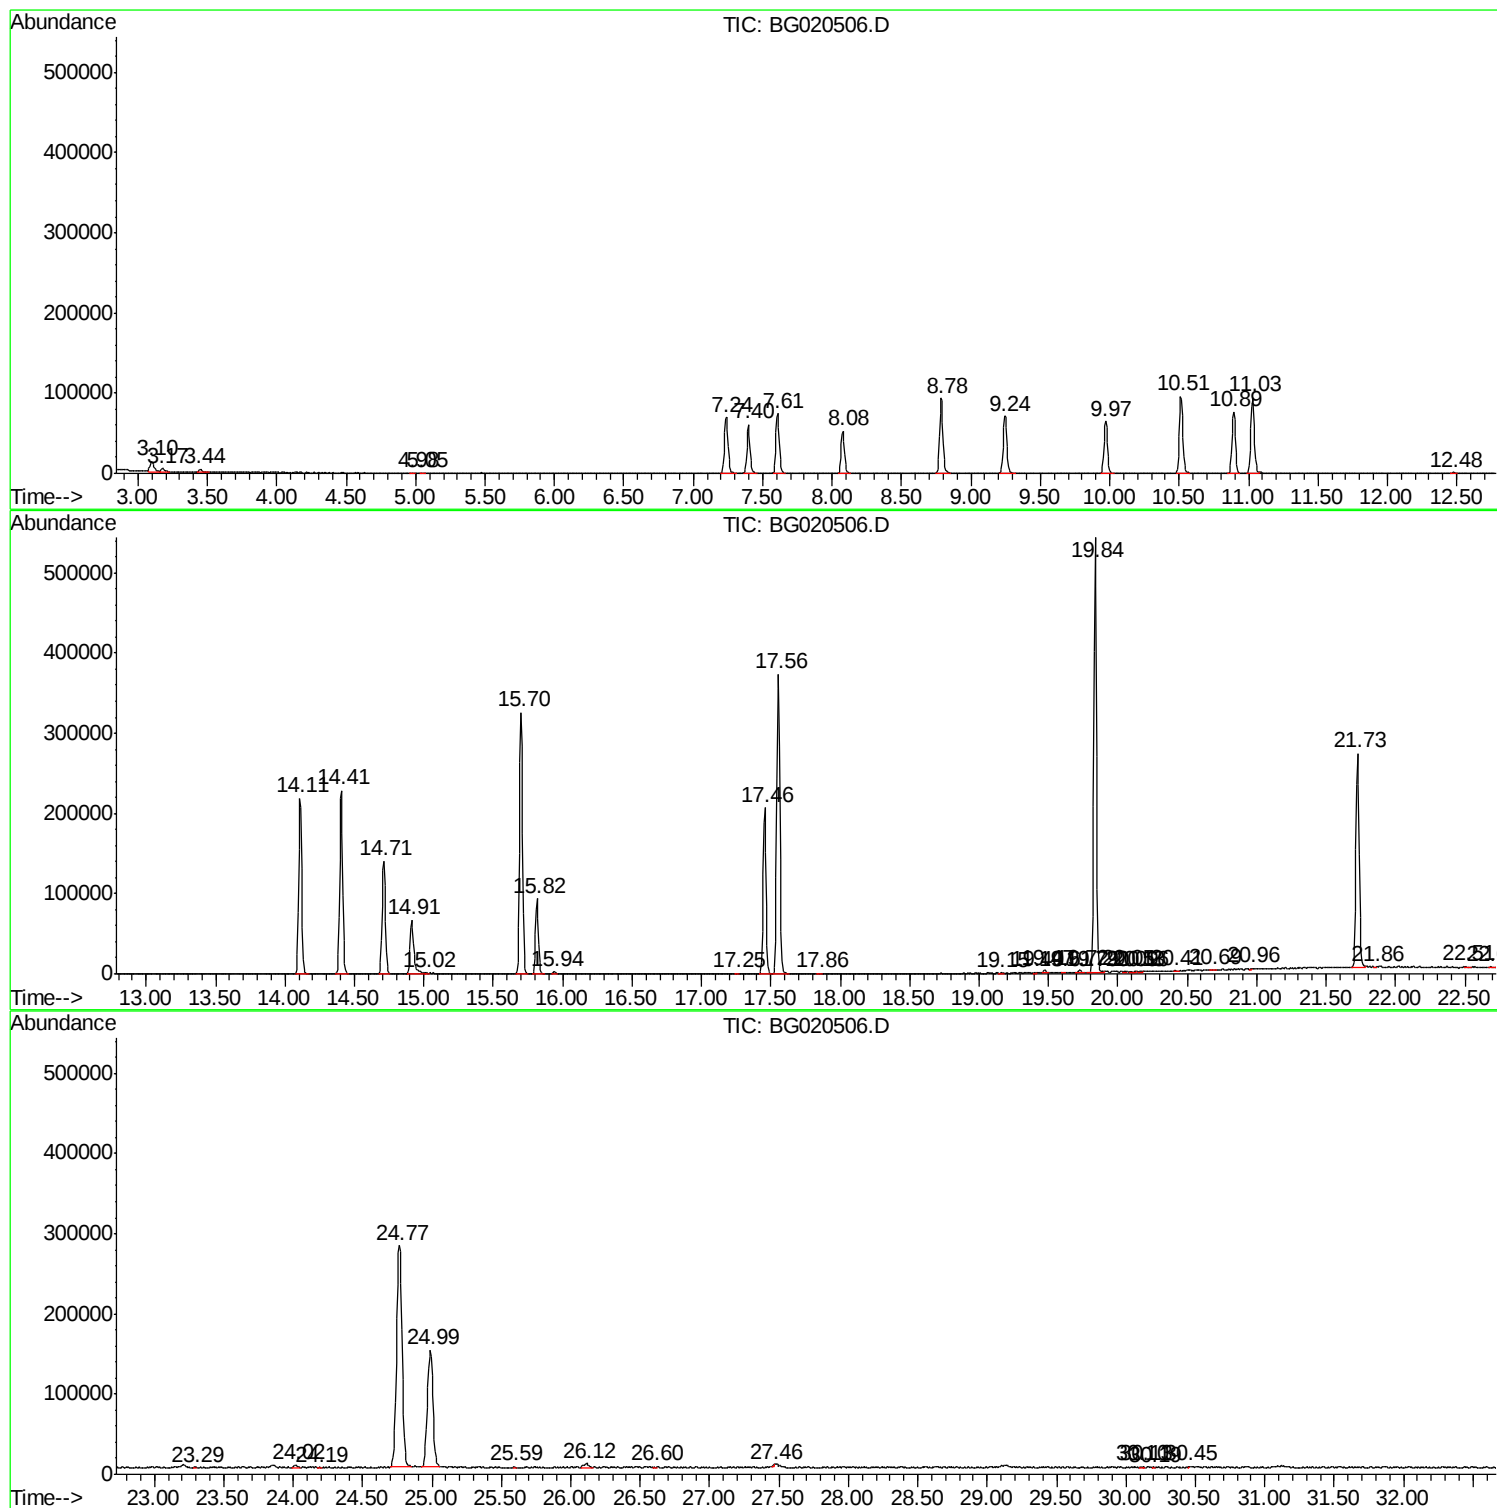

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122515\
Data File : BG020506.D
Acq On : 25 Dec 2015 15:49
Operator : UM/SJ
Sample : PB87434BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK34

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122515\
Data File : BG020506.D
Acq On : 25 Dec 2015 15:49
Operator : UM/SJ
Sample : PB87434BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK34

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc