


Data Path : Z:\HPCHEM1\BNA_G\Data\BG122615\
Data File : BG020546.D
Acq On : 27 Dec 2015 8:44
Operator : UM/SJ
Sample : DFTPP16
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP16

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG122415.M
Title : SVOA CALIBRATION
Last Update : Mon Dec 28 04:59:10 2015

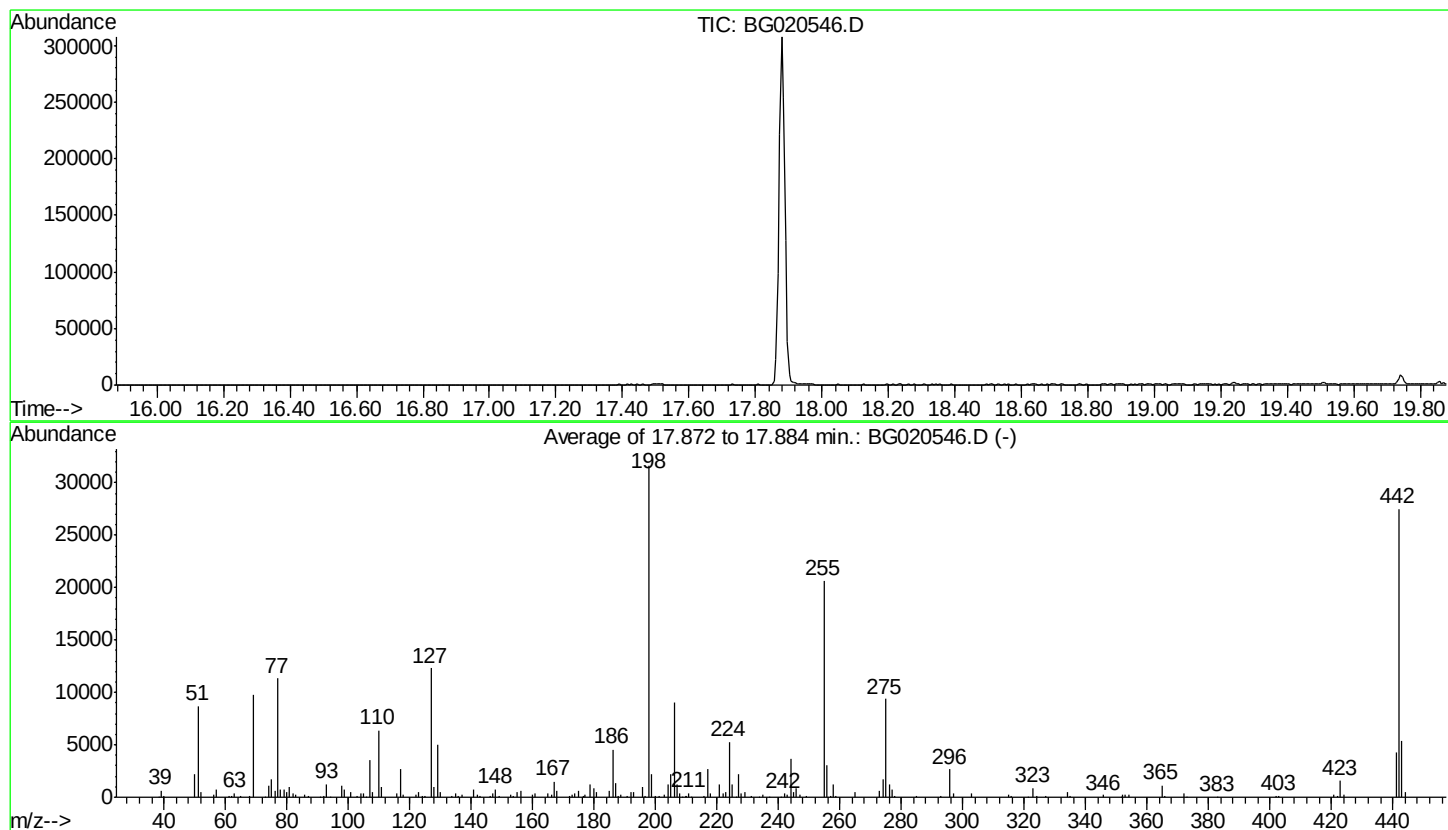

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	8683	PASS
68	69	0.00	2	1.2	120	PASS
69	198	0.00	100	30.7	9715	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.9	12296	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31637	PASS
199	198	5	9	7.0	2200	PASS
275	198	10	60	29.6	9372	PASS
365	198	1	100	3.6	1145	PASS
441	442	0.01	100	15.4	4246	PASS
442	198	50	100	87.0	27538	PASS
443	442	15	24	19.5	5369	PASS

m/z	Abundance
39.00	656.0
44.00	240.0
50.00	2262.0
51.00	8320.0
52.00	428.0
56.00	294.0
56.90	651.0
62.00	155.0
63.00	488.0
65.00	202.0
67.90	181.0
68.90	9220.0
74.00	953.0
75.00	1528.0
76.00	482.0
77.00	10955.0
78.00	679.0
79.00	716.0
80.00	409.0
80.90	914.0
81.90	369.0
83.00	199.0
85.90	276.0
86.90	252.0
93.00	1242.0
97.90	982.0
98.90	847.0
100.90	443.0
103.90	347.0
104.90	293.0
107.00	3050.0
108.00	485.0
109.90	6392.0
110.90	957.0
115.90	262.0
117.00	2302.0
118.00	303.0
121.90	330.0
122.90	456.0
124.90	189.0
127.00	11066.0
128.00	973.0
128.90	4391.0
129.90	435.0
134.90	382.0
137.00	303.0
141.00	608.0
142.00	252.0
143.00	227.0
146.00	198.0
146.90	244.0
147.90	603.0
153.00	222.0
155.00	514.0
156.00	540.0
160.00	245.0
160.90	348.0
164.90	377.0
166.00	233.0
166.90	1322.0
167.90	506.0
172.90	165.0
173.90	237.0
174.90	678.0
176.80	251.0
178.90	1046.0
179.90	735.0
180.90	400.0
184.90	501.0
186.00	4082.0
186.90	1117.0
188.90	172.0
190.90	182.0
191.90	398.0
193.00	450.0
195.90	776.0
197.90	27224.0
198.90	2146.0
199.90	176.0
202.90	291.0
204.00	1082.0
205.00	1750.0
206.00	7433.0
207.00	1012.0
207.90	383.0
209.90	150.0
211.00	293.0
211.70	152.0
216.90	2212.0
217.90	310.0
220.90	1014.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

221.80	345.0
222.90	511.0
224.00	4351.0
225.00	975.0
226.90	2067.0
227.90	268.0
229.00	381.0
231.00	178.0
233.90	158.0
235.00	192.0
240.90	173.0
241.90	267.0
243.00	275.0
244.00	2993.0
245.00	440.0
245.90	695.0
246.90	203.0
248.90	196.0
255.00	17488.0
256.00	2573.0
257.00	183.0
258.00	963.0
264.80	395.0
272.90	563.0
273.90	1399.0
274.90	7537.0
276.00	1032.0
276.90	727.0
295.90	2223.0
296.90	333.0
303.00	319.0
315.00	238.0
315.90	167.0
322.90	621.0
324.10	222.0
334.00	368.0
345.90	181.0
351.80	181.0
352.90	193.0
353.90	202.0
364.90	829.0
371.90	303.0
382.90	163.0
420.90	160.0
422.00	163.0
423.00	911.0
423.90	203.0
441.00	2770.0
442.00	19136.0
443.00	3930.0
444.00	332.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

m/z	Abundance
38.10	166.0
39.00	846.0
40.00	233.0
44.00	290.0
50.00	2494.0
51.00	10570.0
52.00	577.0
56.00	327.0
57.00	880.0
61.00	153.0
62.00	197.0
62.90	438.0
65.00	255.0
68.90	11249.0
73.00	163.0
74.00	1382.0
75.00	2112.0
76.00	816.0
77.00	13249.0
78.00	1000.0
79.00	812.0
80.00	633.0
81.00	1247.0
82.00	358.0
82.90	267.0
86.00	203.0
87.00	182.0
90.90	170.0
91.90	312.0
93.00	1451.0
98.00	1275.0
98.90	820.0
101.00	655.0
102.80	202.0
103.90	341.0
104.90	469.0
105.90	171.0
107.00	4616.0
108.00	531.0
110.00	7431.0
111.00	1232.0
115.90	450.0
117.00	3149.0
118.00	321.0
122.00	369.0
123.00	505.0
124.00	199.0
125.00	273.0
127.00	14687.0
128.00	1328.0
129.00	6090.0
129.90	600.0
133.90	214.0
134.90	460.0
136.00	171.0
136.90	289.0
140.90	903.0
141.90	226.0
142.90	186.0
147.00	425.0
147.90	882.0
149.00	316.0
152.90	396.0
153.90	233.0
154.90	530.0
156.00	598.0
159.90	378.0
161.00	427.0
164.90	276.0
166.00	332.0
167.00	1797.0
167.90	812.0
171.90	208.0
172.90	264.0
173.90	315.0
174.90	628.0
177.00	489.0
178.90	1396.0
179.90	865.0
180.90	482.0
185.00	739.0
186.00	5334.0
187.00	1613.0
188.00	245.0
188.90	303.0
190.90	169.0
191.90	578.0
192.90	578.0
195.90	1368.0
197.90	38096.0
198.90	2543.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

199.90	238.0
201.40	238.0
203.00	320.0
204.00	1482.0
205.00	2628.0
206.00	10740.0
207.00	1451.0
207.90	460.0
208.90	153.0
210.10	254.0
210.90	374.0
215.90	190.0
216.90	3263.0
217.90	457.0
220.90	1597.0
221.90	366.0
222.90	499.0
224.00	6589.0
224.90	1536.0
226.90	2346.0
227.80	377.0
228.90	603.0
234.90	182.0
236.90	188.0
241.90	364.0
243.00	347.0
244.00	4229.0
245.00	645.0
245.90	921.0
246.90	261.0
249.00	167.0
254.90	23120.0
256.00	3443.0
256.80	309.0
257.90	1277.0
258.90	191.0
264.90	464.0
273.00	779.0
274.00	1767.0
275.00	10267.0
276.00	1249.0
276.90	934.0
278.00	260.0
285.00	157.0
292.90	214.0
296.00	3127.0
296.90	435.0
303.00	385.0
315.00	281.0
315.90	164.0
323.00	1078.0
324.00	172.0
326.90	170.0
333.90	488.0
335.00	196.0
345.90	271.0
352.00	413.0
353.00	157.0
354.00	326.0
364.90	1261.0
366.00	207.0
371.90	515.0
402.00	207.0
403.00	277.0
421.00	219.0
421.90	204.0
423.00	1840.0
423.90	339.0
441.00	5073.0
442.00	30624.0
443.00	5957.0
444.00	539.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

m/z	Abundance
39.00	436.0
43.90	217.0
50.00	1807.0
51.00	7160.0
52.00	357.0
56.00	224.0
57.00	604.0
61.00	170.0
61.90	163.0
63.00	367.0
67.90	180.0
69.00	8678.0
74.00	872.0
74.90	1444.0
76.10	536.0
77.00	9703.0
78.00	695.0
79.00	504.0
80.00	488.0
80.90	752.0
82.00	216.0
82.90	212.0
86.00	229.0
92.90	1058.0
94.00	166.0
97.90	982.0
98.90	724.0
101.00	255.0
102.90	180.0
104.00	337.0
104.90	209.0
107.00	2905.0
107.90	511.0
109.90	5369.0
110.90	722.0
116.00	247.0
116.90	2521.0
117.90	224.0
121.90	190.0
122.90	335.0
123.90	152.0
127.00	11137.0
127.90	795.0
129.00	4693.0
129.90	379.0
133.90	163.0
134.90	308.0
135.90	159.0
140.90	622.0
141.90	214.0
146.90	331.0
148.00	822.0
148.90	209.0
152.90	294.0
153.90	186.0
154.90	416.0
156.00	766.0
159.80	211.0
160.90	337.0
165.00	295.0
166.00	256.0
166.90	1312.0
168.00	576.0
173.00	164.0
173.90	378.0
175.00	585.0
176.00	170.0
176.90	217.0
178.90	1066.0
179.90	874.0
181.00	475.0
184.90	653.0
186.00	4160.0
187.00	1388.0
188.90	235.0
191.00	197.0
192.00	328.0
192.90	418.0
196.00	933.0
196.60	303.0
197.90	29592.0
198.90	1911.0
202.90	278.0
204.00	1200.0
205.00	2049.0
206.00	8836.0
207.00	1183.0
208.00	302.0
209.80	171.0
210.90	491.0
216.00	263.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

216.90	2446.0
217.90	353.0
220.90	1237.0
221.90	353.0
223.00	602.0
224.00	4895.0
224.90	1235.0
226.00	173.0
226.90	2020.0
227.90	315.0
228.90	464.0
231.00	173.0
234.90	254.0
241.90	332.0
242.90	275.0
244.00	3772.0
244.90	559.0
245.90	847.0
247.00	156.0
254.90	21392.0
255.90	3100.0
257.90	1382.0
258.90	201.0
264.90	462.0
272.90	641.0
273.90	1925.0
275.00	10313.0
276.00	1499.0
276.90	722.0
284.90	183.0
292.90	215.0
295.90	2555.0
296.90	362.0
302.90	275.0
314.90	267.0
316.00	177.0
321.00	155.0
322.90	881.0
326.80	153.0
334.00	661.0
335.00	238.0
345.80	259.0
351.90	297.0
353.00	251.0
353.90	308.0
364.90	1347.0
365.90	162.0
372.00	410.0
372.80	186.0
402.90	198.0
421.00	330.0
423.00	1849.0
423.90	283.0
441.00	4896.0
442.00	32856.0
443.00	6220.0
443.90	453.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16

m/z	Abundance
44.00	288.0

Instrument :
BNA_G
ClientSampleId :
DFTPP16