


Data Path : U:\HPCHEM1\BNA G\Data\BG122617\
 Data File : BG031755.D
 Acq On : 26 Dec 2017 10:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

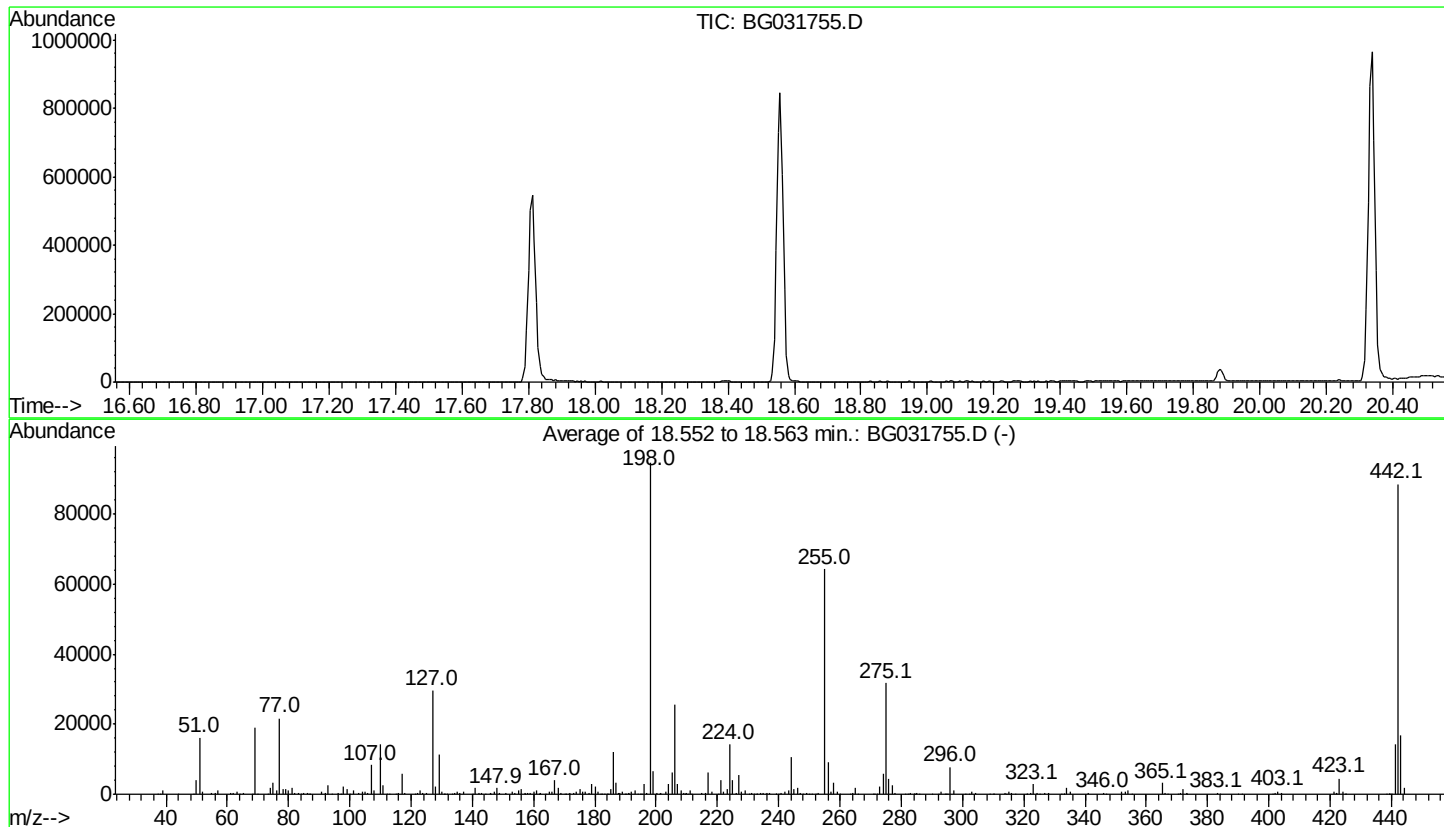

AutoFind: Scans 2598, 2599, 2600; Background Corrected with Scan 2591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.0	16125	PASS
68	69	0.00	2	0.7	130	PASS
69	198	0.00	100	19.9	18877	PASS
70	69	0.00	2	0.8	145	PASS
127	198	10	80	31.3	29586	PASS
197	198	0.00	2	0.3	318	PASS
198	198	100	100	100.0	94672	PASS
199	198	5	9	7.0	6646	PASS
275	198	10	60	33.5	31674	PASS
365	198	1	100	3.5	3267	PASS
441	442	0.01	24	16.0	14135	PASS
442	198	50	100	93.5	88565	PASS
443	442	15	24	19.1	16959	PASS