


Data Path : U:\HPCHEM1\BNA G\Data\BG122617\  
 Data File : BG031774.D  
 Acq On : 26 Dec 2017 23:30  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG122117.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Dec 22 11:08:55 2017

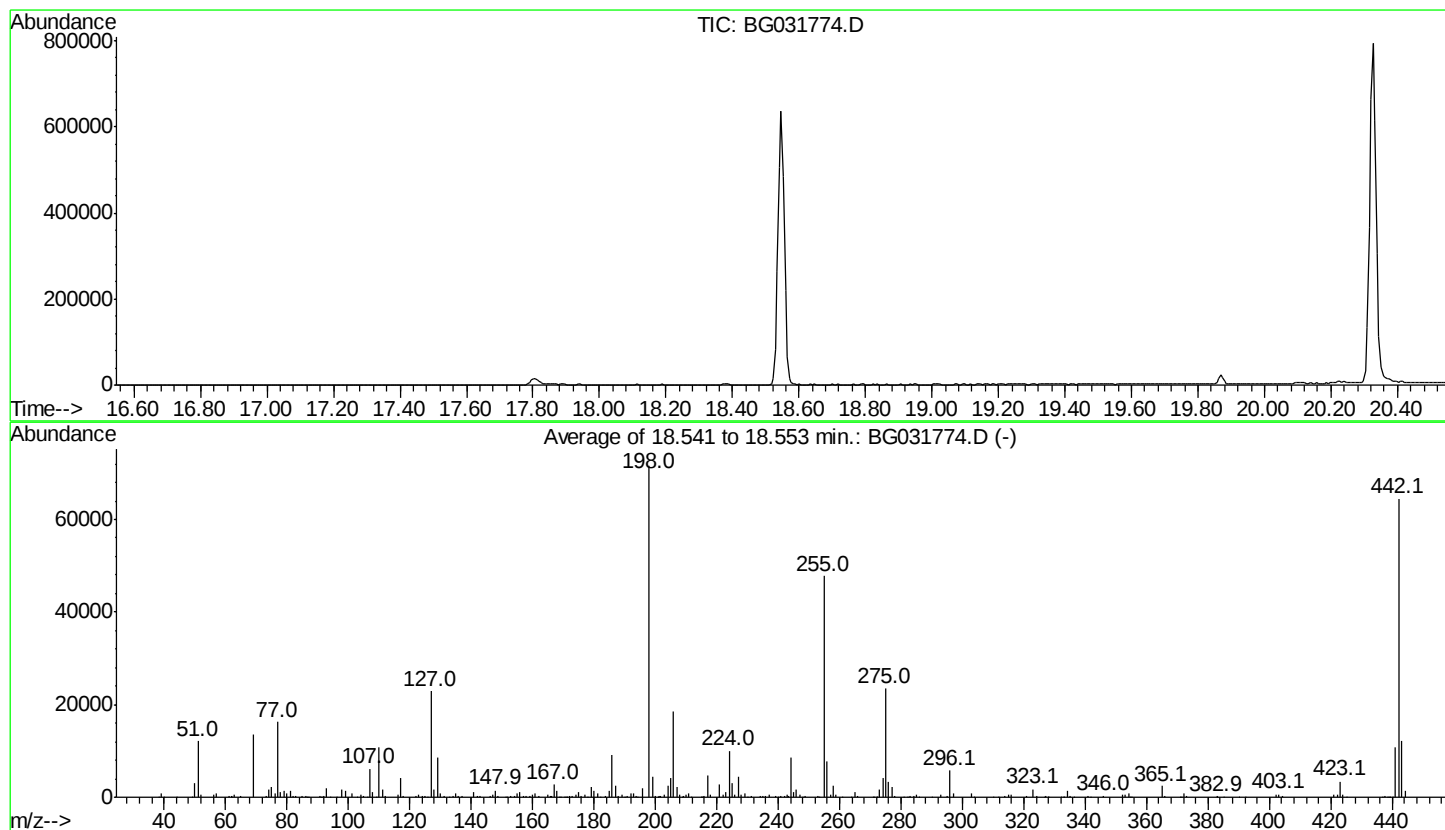

AutoFind: Scans 2596, 2597, 2598; Background Corrected with Scan 2589

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 16.9      | 12111   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 19.0      | 13633   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 31.9      | 22866   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 71626   | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 4541    | PASS             |
| 275         | 198          | 10           | 60           | 32.8      | 23464   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 2483    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.6      | 10716   | PASS             |
| 442         | 198          | 50           | 100          | 90.0      | 64493   | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 12243   | PASS             |