

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122623\
 Data File : BG060174.D
 Acq On : 26 Dec 2023 17:49
 Operator : MA/JU
 Sample : PB158041BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB158041BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.508	405	412	430	rBV	4899077	7685787	32.22%	8.377%
2	7.100	675	683	702	rBV	5116414	8948449	37.51%	9.753%
3	7.940	817	826	834	rBV	598814	1049396	4.40%	1.144%
4	9.104	1015	1024	1036	rBV	2587002	4714505	19.76%	5.138%
5	10.743	1295	1303	1314	rBV	957969	1703913	7.14%	1.857%
6	13.199	1713	1721	1738	rBV	8142551	13130419	55.04%	14.310%
7	14.574	1946	1955	1965	rBV	1939521	3060812	12.83%	3.336%
8	16.066	2201	2209	2229	rBV	7325789	11445449	47.98%	12.474%
9	17.323	2416	2423	2433	rBV	3045364	4561369	19.12%	4.971%
10	19.944	2862	2869	2881	rBV	16249539	23854649	100.00%	25.998%
11	21.589	3142	3149	3166	rVB	3124199	5318973	22.30%	5.797%
12	24.227	3592	3598	3611	rVB5	103322	273852	1.15%	0.298%
13	24.762	3679	3689	3703	rBV2	1858073	5433659	22.78%	5.922%
14	25.496	3807	3814	3826	rVB5	92682	310014	1.30%	0.338%
15	27.071	4074	4082	4091	rBV8	78007	262877	1.10%	0.287%




Sum of corrected areas: 91754123

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122623\
Data File : BG060174.D
Acq On : 26 Dec 2023 17:49
Operator : MA/JU
Sample : PB158041BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

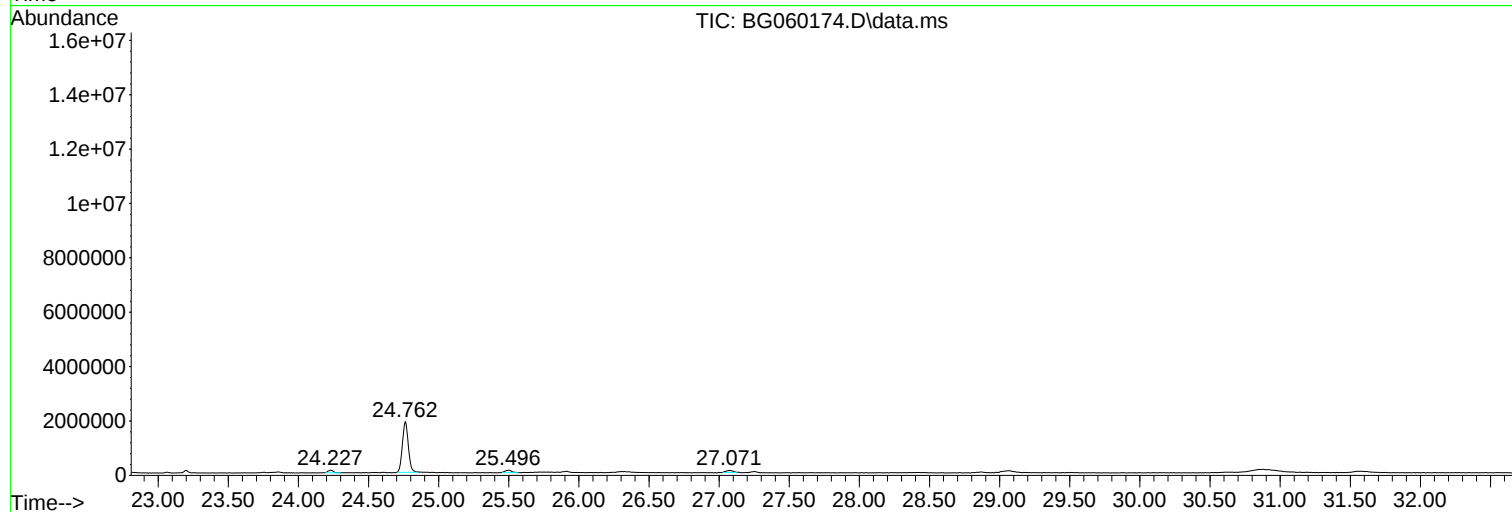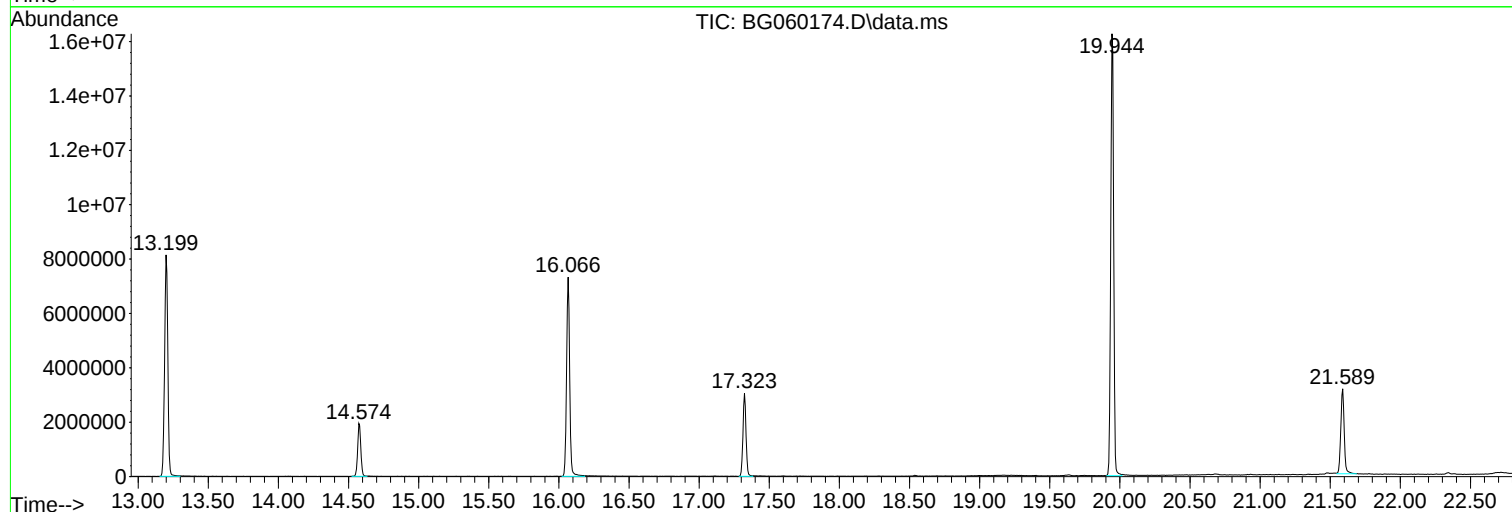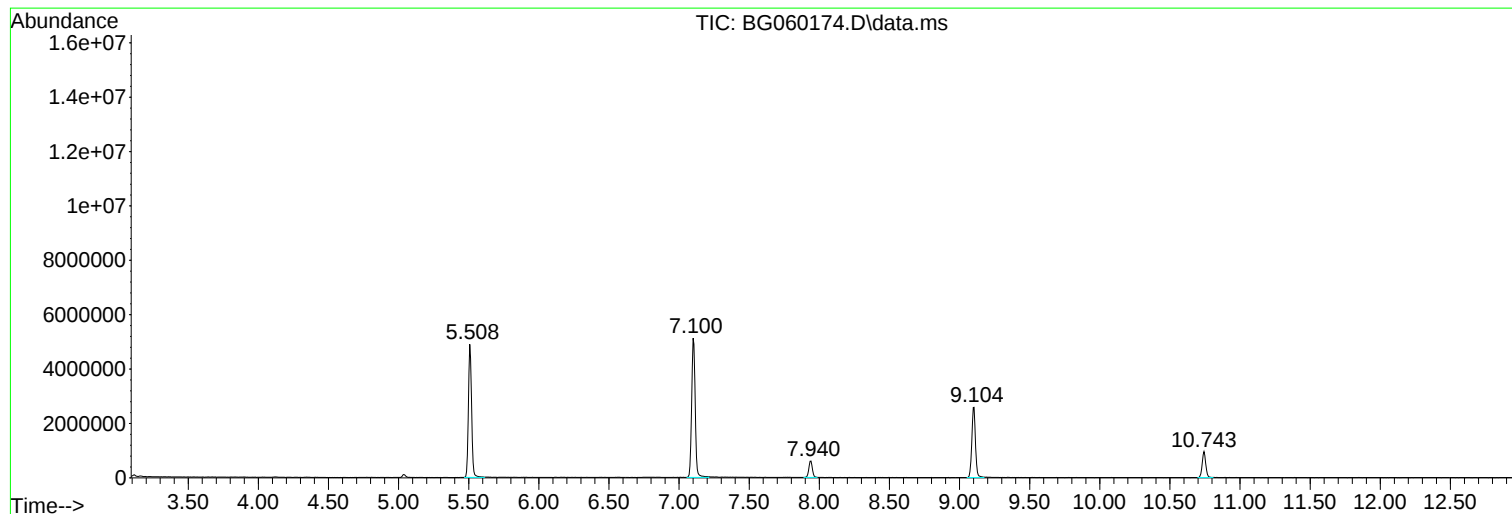

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122623\
Data File : BG060174.D
Acq On : 26 Dec 2023 17:49
Operator : MA/JU
Sample : PB158041BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122623\
Data File : BG060174.D
Acq On : 26 Dec 2023 17:49
Operator : MA/JU
Sample : PB158041BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------