
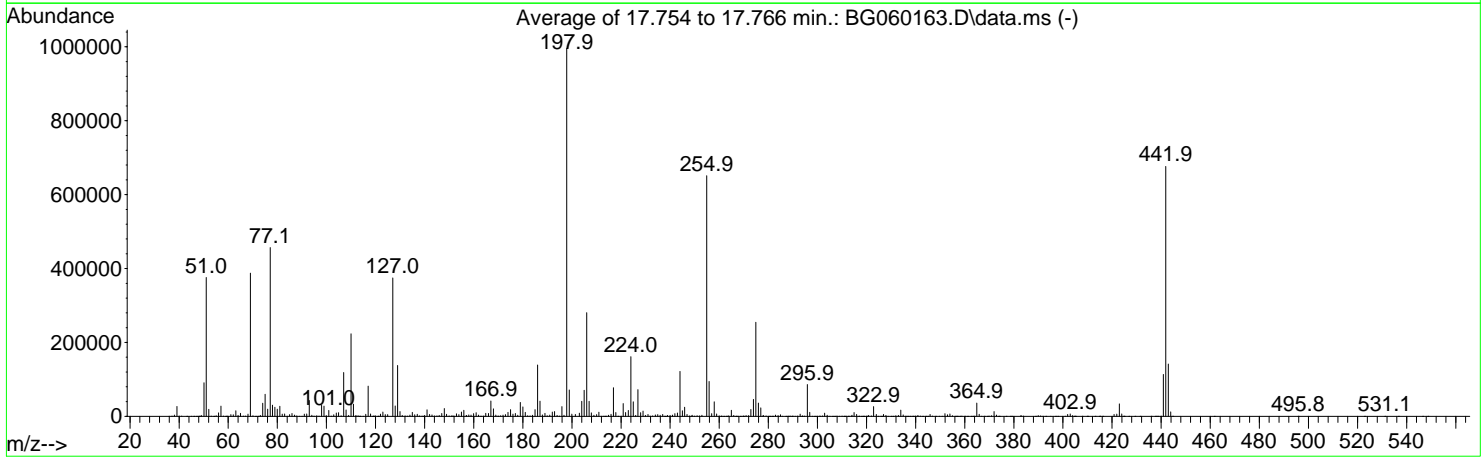


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122623\  
 Data File : BG060163.D  
 Acq On : 26 Dec 2023 8:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122623.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Dec 27 00:45:31 2023

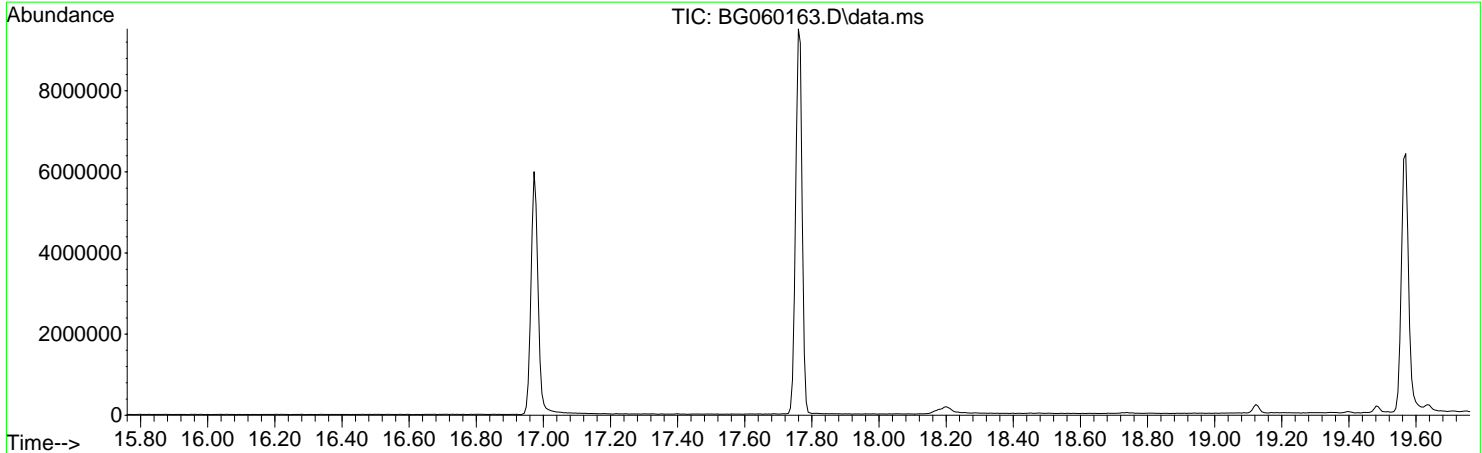




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	375695	PASS
68	69	0.00	2	1.5	5934	PASS
69	198	0.00	100	38.9	387467	PASS
70	69	0.00	2	0.4	1547	PASS
127	198	10	80	37.6	374613	PASS
197	198	0.00	2	0.3	3141	PASS
198	198	100	100	100.0	995371	PASS
199	198	5	9	7.2	71443	PASS
275	198	10	60	25.6	254677	PASS
365	198	1	100	3.6	35856	PASS
441	198	0.01	100	11.4	113424	PASS
442	442	50	100	100.0	676309	PASS
443	442	15	24	20.9	141413	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122623\  
 Data File : BG060163.D  
 Acq On : 26 Dec 2023 8:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Quant Time: Dec 27 00:52:36 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122623.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 27 00:45:31 2023  
 Response via : Initial Calibration

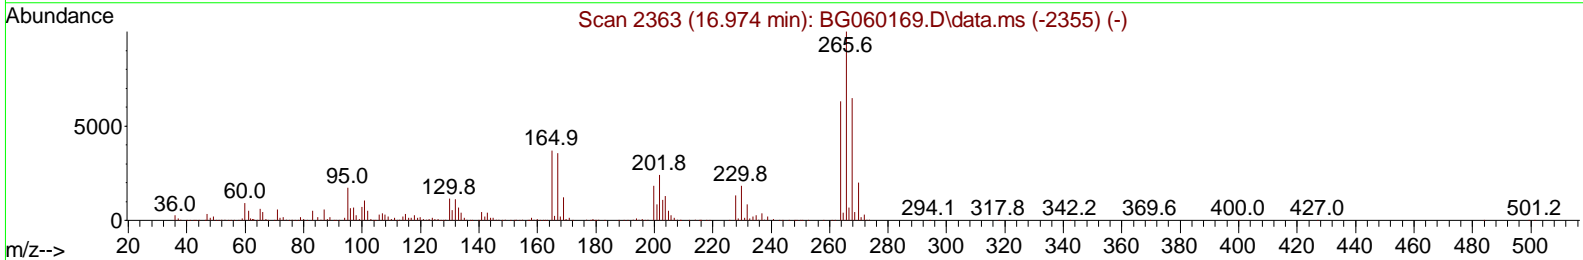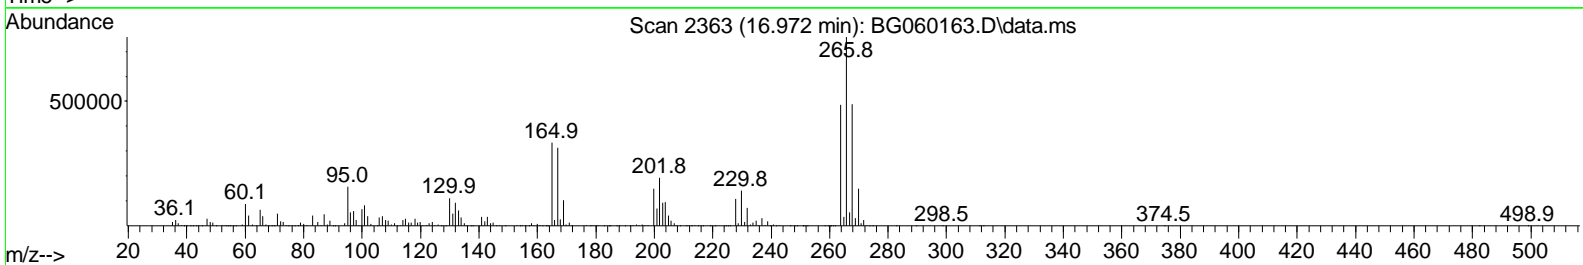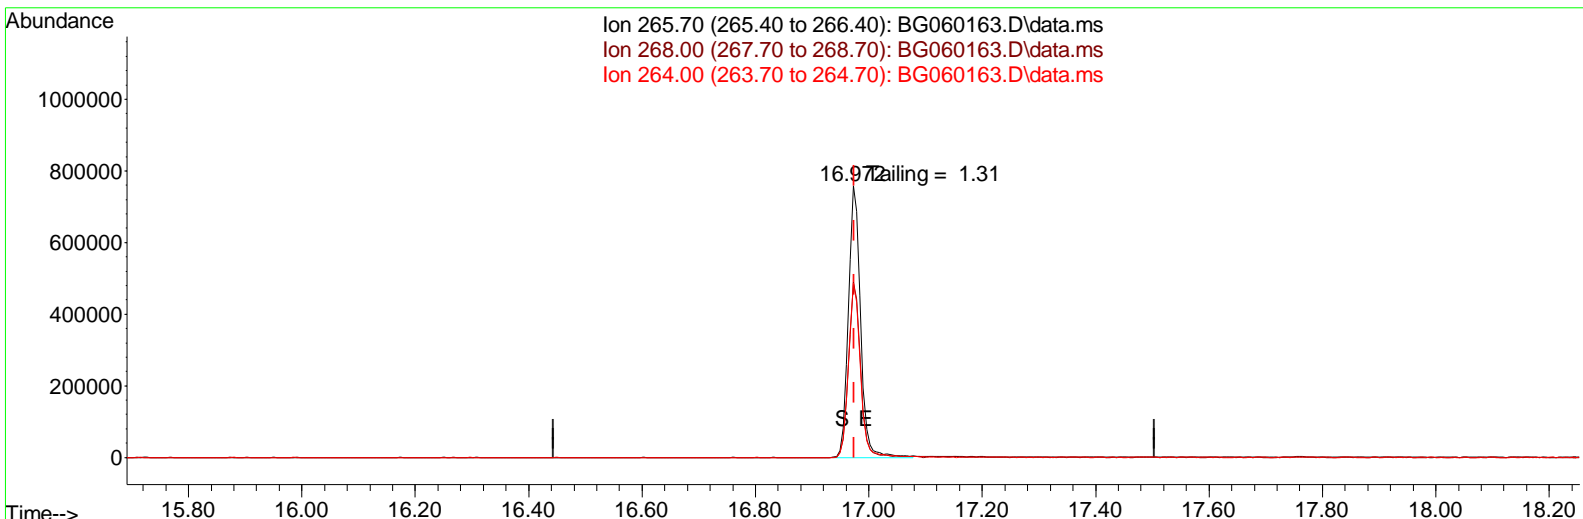

TIC: BG060163.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.002) 1018815.21 ng




response 1143102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.30	64.50
264.00	67.10	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122623\  
 Data File : BG060163.D  
 Acq On : 26 Dec 2023 8:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Quant Time: Dec 27 00:52:36 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122623.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 27 00:45:31 2023  
 Response via : Initial Calibration

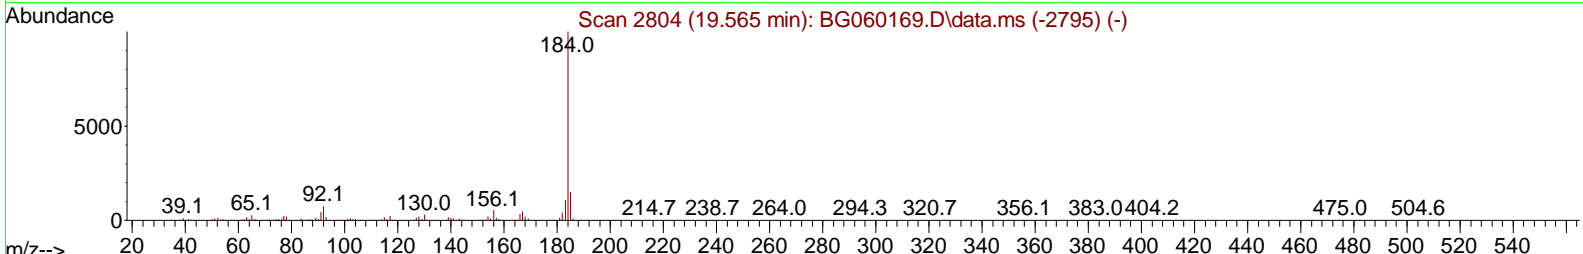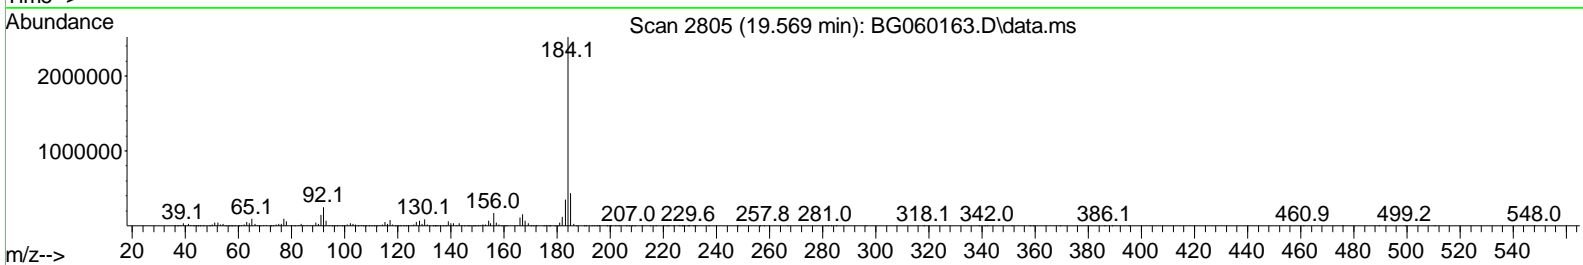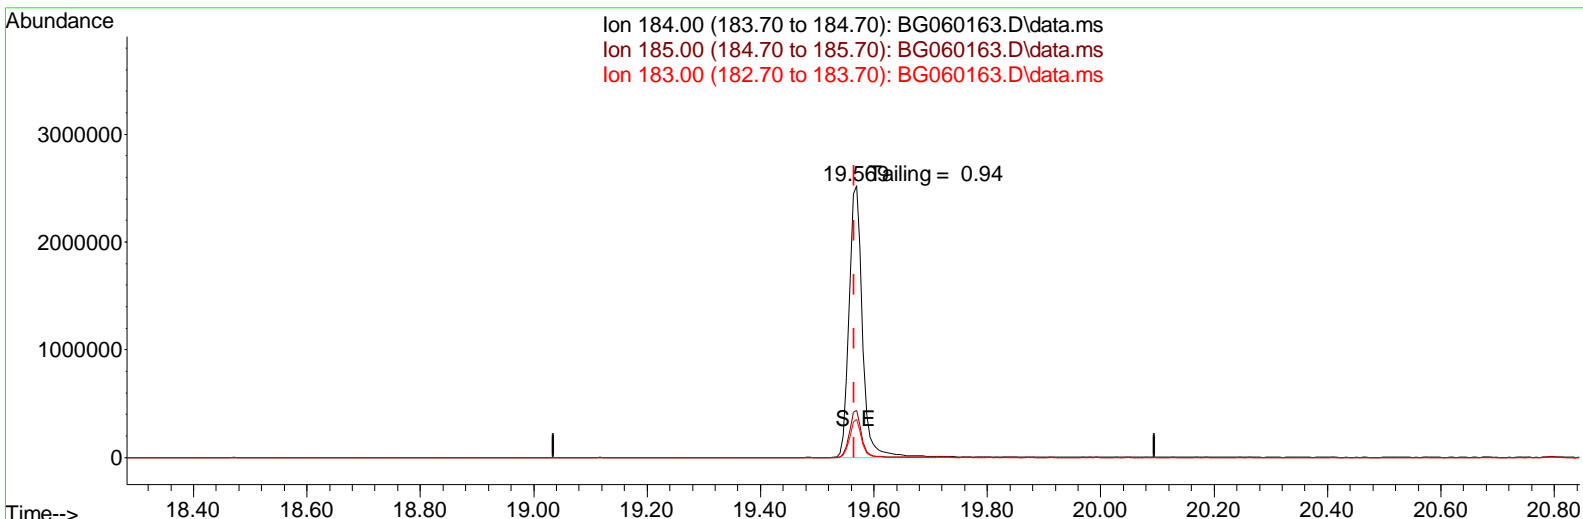

TIC: BG060163.D\data.ms

(77) Benzidine

19.569min (+ 0.004) 15902.10 ng

response 4164522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	17.39
183.00	10.80	14.04#
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
12/26/2023	BNA_G	<u>BG060163.D</u>
Compound Name	Response	Retention Time
DDT	2178451	20.797
DDD	138843	20.357
DDE	2671	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
141514	2319965	6.10

Instrument :  
 BNA\_G  
 ClientSampled :  
 DFTPP