

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063913.D
 Acq On : 28 Dec 2024 21:38
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc : SPIKE
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020589

Quant Time: Dec 29 23:28:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 00:44:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	107012	20.000	ng/u1	0.00
20) Naphthalene-d8	10.585	136	444584	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	329320	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.195	188	793567	20.000	ng/u1	0.00
79) Chrysene-d12	21.449	240	798473	20.000	ng/u1	# 0.01
88) Perylene-d12	24.469	264	818917	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.259	96	23531	8.617	ng/uL	0.00
4) Pyridine-d5	3.664	84	176452	20.483	ng/u1	0.00
7) Phenol-d5	6.984	99	196001	19.887	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.125	67	128717	18.909	ng/u1	0.00
11) 2-Chlorophenol-d4	7.336	132	127316	19.954	ng/u1	0.00
15) 4-Methylphenol-d8	8.517	113	147797	19.315	ng/u1	0.00
21) Nitrobenzene-d5	8.952	128	68345	21.530	ng/u1	0.00
24) 2-Nitrophenol-d4	9.675	143	75398	21.189	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.221	165	153526	22.285	ng/u1	0.00
31) 4-Chloroaniline-d4	10.726	131	191744	21.920	ng/u1	0.00
46) Dimethylphthalate-d6	13.846	166	472674	21.093	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	553864	21.682	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	58574	18.448	ng/u1	0.00
60) Fluorene-d10	15.439	176	436856	22.049	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	67914	16.483	ng/u1	0.01
73) Anthracene-d10	17.295	188	764736	22.414	ng/u1	0.00
81) Pyrene-d10	19.598	212	872469	20.998	ng/u1	0.01
92) Benzo(a)pyrene-d12	24.269	264	837194	21.770	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.294	88	28412	8.792	ng/uL	89
5) Pyridine	3.682	79	192597	20.873	ng/u1	97
6) Benzaldehyde	6.937	77	236670	39.148	ng/u1	95
8) Phenol	7.013	94	207617	19.766	ng/u1	91
10) Bis(2-Chloroethyl)ether	7.219	93	158972	19.781	ng/u1	96
12) 2-Chlorophenol	7.366	128	135463	20.974	ng/u1	99
13) 2-Methylphenol	8.253	108	150911	19.878	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.312	45	233144	19.542	ng/u1	98
16) Acetophenone	8.617	105	254498	19.609	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.600	70	141872	18.320	ng/u1	92
18) 4-Methylphenol	8.576	108	164892	19.845	ng/u1	99
19) Hexachloroethane	8.870	117	58607	18.467	ng/u1	92
22) Nitrobenzene	8.993	77	210805	19.887	ng/u1	97
23) Isophorone	9.516	82	389142	19.429	ng/u1	98
25) 2-Nitrophenol	9.704	139	78172	21.377	ng/u1	91
26) 2,4-Dimethylphenol	9.775	107	163900	19.751	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.998	93	224367	20.711	ng/u1	97
29) 2,4-Dichlorophenol	10.251	162	151272	22.099	ng/u1	92
30) Naphthalene	10.638	128	461508	20.763	ng/u1	98
32) 4-Chloroaniline	10.750	127	187327	22.508	ng/u1	97
33) Hexachlorobutadiene	10.920	225	107020	19.244	ng/u1	95
34) Caprolactam	11.496	113	39589	16.730	ng/u1	90
35) 4-Chloro-3-methylphenol	11.896	107	166706	20.743	ng/u1	97
36) 2-Methylnaphthalene	12.254	142	329858	20.648	ng/u1	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063913.D
 Acq On : 28 Dec 2024 21:38
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc : SPIKE
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020589

Quant Time: Dec 29 23:28:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 00:44:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.471	142	338949	20.829	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.624	216	214296	20.327	ng/ul	98
40) Hexachlorocyclopentadiene	12.601	237	42555	10.211	ng/ul	90
41) 2,4,6-Trichlorophenol	12.877	196	125534	21.068	ng/ul	95
42) 2,4,5-Trichlorophenol	12.953	196	133524	21.472	ng/ul	97
43) 1,1'-Biphenyl	13.270	154	467970	21.547	ng/ul	96
44) 2-Chloronaphthalene	13.312	162	371235	21.286	ng/ul	95
45) 2-Nitroaniline	13.523	65	127109	21.759	ng/ul	95
47) Dimethylphthalate	13.893	163	477389	21.257	ng/ul	97
48) 2,6-Dinitrotoluene	14.023	165	97837	23.457	ng/ul#	87
50) Acenaphthylene	14.164	152	597255	21.805	ng/ul	100
51) 3-Nitroaniline	14.352	138	80615	20.905	ng/ul	82
52) Acenaphthene	14.504	153	420127	21.641	ng/ul	95
53) 2,4-Dinitrophenol	14.587	184	20016	9.390	ng/ul	88
55) 4-Nitrophenol	14.686	109	54604	16.562	ng/ul	94
56) Dibenzofuran	14.845	168	597556	21.832	ng/ul	94
57) 2,4-Dinitrotoluene	14.822	165	147887	23.862	ng/ul	93
58) 2,3,4,6-Tetrachlorophenol	15.080	232	112738	21.032	ng/ul	95
59) Diethylphthalate	15.268	149	473196	21.795	ng/ul	99
61) Fluorene	15.497	166	481709	22.041	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.486	204	258370	21.220	ng/ul	95
63) 4-Nitroaniline	15.521	138	69621	18.033	ng/ul	91
66) 4,6-Dinitro-2-methylph...	15.591	198	71139	16.759	ng/ul#	88
67) N-Nitrosodiphenylamine	15.703	169	421763	21.948	ng/ul	99
68) 4-Bromophenyl-phenylether	16.384	248	173535	21.457	ng/ul	99
69) Hexachlorobenzene	16.508	284	194644	21.481	ng/ul	99
70) Atrazine	16.661	200	175372	21.589	ng/ul	96
71) Pentachlorophenol	16.866	266	51640	13.517	ng/ul	91
72) Phenanthrene	17.236	178	862424	22.552	ng/ul	99
74) Anthracene	17.330	178	874539	22.594	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.235	216	214051	20.217	ng/ul	97
76) Pentachlorobenzene	14.769	250	221780	21.144	ng/ul	98
77) Carbazole	17.607	167	738984	23.586	ng/ul	98
78) Di-n-butylphthalate	18.165	149	888705	23.487	ng/ul	98
80) Fluoranthene	19.263	202	1020278	21.604	ng/ul	99
82) Pyrene	19.628	202	1106258	22.017	ng/ul	97
83) Butylbenzylphthalate	20.521	149	357063	23.150	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.349	252	301235	20.899	ng/ul	92
85) Benzo(a)anthracene	21.432	228	1046298	20.909	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.343	149	546663	24.365	ng/ul	99
87) Chrysene	21.496	228	989372	20.744	ng/ul	99
89) Di-n-octyl phthalate	22.477	149	898860	25.430	ng/ul	100
90) Benzo(b)fluoranthene	23.517	252	1007473	21.646	ng/ul	98
91) Benzo(k)fluoranthene	23.517	252	1007473	21.700	ng/ul	97
93) Benzo(a)pyrene	24.328	252	934887	21.400	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	27.871	276	1184514	22.202	ng/ul	100
95) Dibenzo(a,h)anthracene	27.930	278	939672	22.011	ng/ul	94
96) Benzo(g,h,i)perylene	28.946	276	924159	21.829	ng/ul	95





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 8.792 ng/uL
RT: 3.294 min Scan# 31
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion: 88 Resp: 28412
Ion Ratio Lower Upper
88 100
43 29.6 20.9 31.3
58 61.2 57.7 86.5

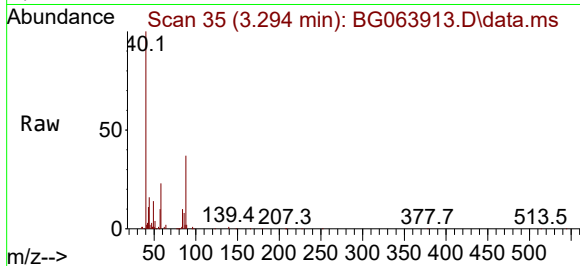

#5
Pyridine
Concen: 20.873 ng/uL
RT: 3.682 min Scan# 101
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion: 79 Resp: 192597
Ion Ratio Lower Upper
79 100
52 77.4 60.9 91.3
51 33.8 29.5 44.3




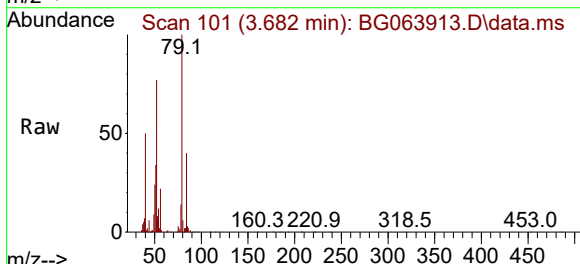




#6
Benzaldehyde
Concen: 39.148 ng/ul
RT: 6.937 min Scan# 61
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion: 77 Resp: 236670
Ion Ratio Lower Upper
77 100
105 86.7 65.2 97.8
106 79.8 61.0 91.4



#8
Phenol
Concen: 19.766 ng/ul
RT: 7.013 min Scan# 668
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion: 94 Resp: 207617
Ion Ratio Lower Upper
94 100
65 27.9 25.6 38.4
66 36.5 34.2 51.2









#10
Bis(2-Chloroethyl)ether
Concen: 19.781 ng/ul
RT: 7.219 min Scan# 703
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion: 93 Resp: 158972
Ion Ratio Lower Upper
93 100
63 83.6 63.8 95.6
95 32.2 27.6 41.4



#12
2-Chlorophenol
Concen: 20.974 ng/ul
RT: 7.366 min Scan# 728
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:128 Resp: 135463
Ion Ratio Lower Upper
128 100
64 60.5 48.9 73.3
130 30.5 24.2 36.2









#13
2-Methylphenol
Concen: 19.878 ng/ul
RT: 8.253 min Scan# 81
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:108 Resp: 150911
Ion Ratio Lower Upper
108 100
107 90.5 72.6 108.8



#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.542 ng/ul
RT: 8.312 min Scan# 889
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion: 45 Resp: 233144
Ion Ratio Lower Upper
45 100
77 13.6 11.5 17.3
79 10.5 9.2 13.8



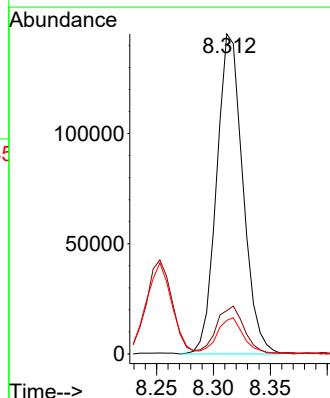





#16
Acetophenone
Concen: 19.609 ng/ul
RT: 8.617 min Scan# 941
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:105 Resp: 254498
Ion Ratio Lower Upper
105 100
77 90.4 73.6 110.4
51 27.3 25.4 38.2



#17
N-Nitroso-di-n-propylamine
Concen: 18.320 ng/ul
RT: 8.600 min Scan# 938
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion: 70 Resp: 141872
Ion Ratio Lower Upper
70 100
42 51.5 47.4 71.0
101 8.3 6.1 9.1
130 12.8 11.4 17.2









#18
4-Methylphenol
Concen: 19.845 ng/ul
RT: 8.576 min Scan# 911
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:108 Resp: 164892
Ion Ratio Lower Upper
108 100
107 112.3 89.2 133.8

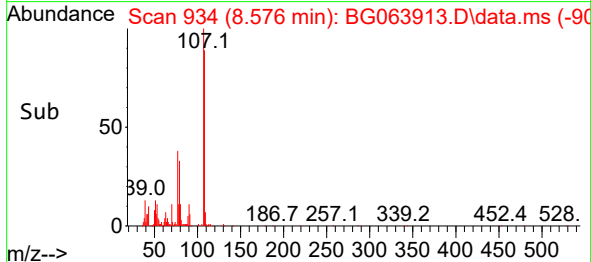

#19
Hexachloroethane
Concen: 18.467 ng/ul
RT: 8.870 min Scan# 984
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:117 Resp: 58607
Ion Ratio Lower Upper
117 100
201 119.7 86.8 130.2
199 77.5 59.4 89.2




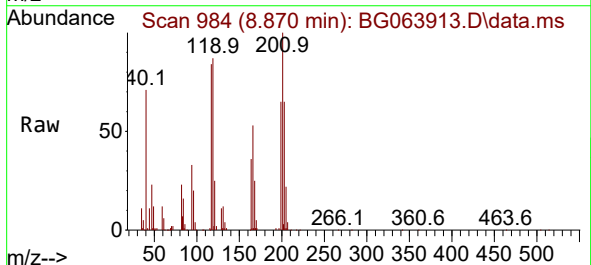




#22
Nitrobenzene
Concen: 19.887 ng/ul
RT: 8.993 min Scan# 1005
Delta R.T. -0.005 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion: 77 Resp: 210805
Ion Ratio Lower Upper
77 100
123 32.3 27.0 40.4
65 12.1 10.8 16.2



#23
Isophorone
Concen: 19.429 ng/ul
RT: 9.516 min Scan# 1094
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion: 82 Resp: 389142
Ion Ratio Lower Upper
82 100
95 6.3 5.8 8.6
138 13.5 10.3 15.5









#25
2-Nitrophenol
Concen: 21.377 ng/ul
RT: 9.704 min Scan# 1126
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:139 Resp: 78172
Ion Ratio Lower Upper
139 100
65 69.8 62.2 93.2
109 37.8 26.9 40.3



#26
2,4-Dimethylphenol
Concen: 19.751 ng/ul
RT: 9.775 min Scan# 1138
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:107 Resp: 163900
Ion Ratio Lower Upper
107 100
121 46.4 38.4 57.6
122 77.5 61.8 92.8





#27

Bis(2-Chloroethoxy)methane

Concen: 20.711 ng/ul

RT: 9.998 min Scan# 1176

Delta R.T. 0.001 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion: 93 Resp: 224367

Ion Ratio Lower Upper

93 100

95 30.6 23.5 35.3

123 9.2 6.2 9.4

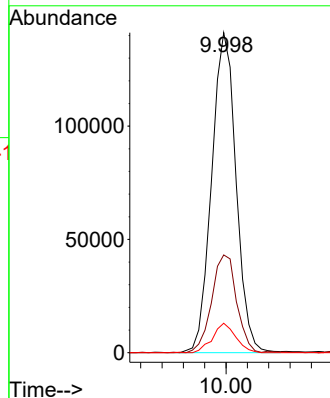

#29

2,4-Dichlorophenol

Concen: 22.099 ng/ul

RT: 10.251 min Scan# 1219

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:162 Resp: 151272


Ion Ratio Lower Upper

162 100

164 61.8 53.0 79.4

98 33.3 33.0 49.6



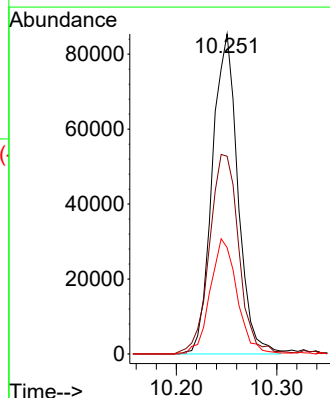





#30
Naphthalene
Concen: 20.763 ng/ul
RT: 10.638 min Scan# 1285
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:128 Resp: 461508
Ion Ratio Lower Upper
128 100
129 11.1 8.2 12.2
127 13.3 9.8 14.8



#32
4-Chloroaniline
Concen: 22.508 ng/ul
RT: 10.750 min Scan# 1304
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:127 Resp: 187327
Ion Ratio Lower Upper
127 100
129 32.2 24.5 36.7









#33
Hexachlorobutadiene
Concen: 19.244 ng/ul
RT: 10.920 min Scan# 11
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:225 Resp: 107020
Ion Ratio Lower Upper
225 100
223 67.5 51.2 76.8
227 67.9 51.1 76.7



#34
Caprolactam
Concen: 16.730 ng/ul
RT: 11.496 min Scan# 1431
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:113 Resp: 39589
Ion Ratio Lower Upper
113 100
55 179.3 162.3 243.5
56 134.7 107.1 160.7




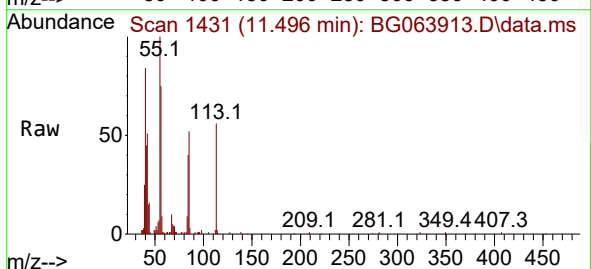




#35
4-Chloro-3-methylphenol
Concen: 20.743 ng/ul
RT: 11.896 min Scan# 1499
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:107 Resp: 166706
Ion Ratio Lower Upper
107 100
144 23.7 16.3 24.5
142 69.7 55.0 82.4



#36
2-Methylnaphthalene
Concen: 20.648 ng/ul
RT: 12.254 min Scan# 1560
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:142 Resp: 329858
Ion Ratio Lower Upper
142 100
141 90.7 69.5 104.3





#37

1-Methylnaphthalene

Concen: 20.829 ng/ul

RT: 12.471 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:142 Resp: 338949

Ion Ratio Lower Upper

142 100

141 96.3 73.8 110.6

116 4.1 3.5 5.3

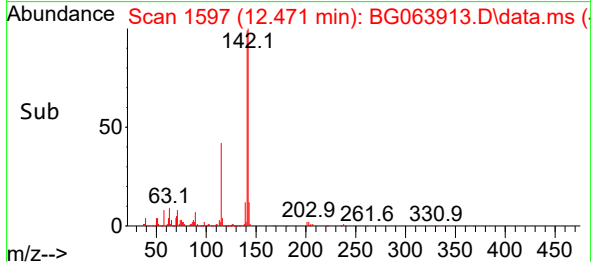

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.327 ng/ul

RT: 12.624 min Scan# 1623

Delta R.T. 0.001 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Tgt Ion:216 Resp: 214296




Ion Ratio Lower Upper


216 100

214 79.0 62.6 93.8

179 18.9 16.5 24.7

108 15.5 11.2 16.8



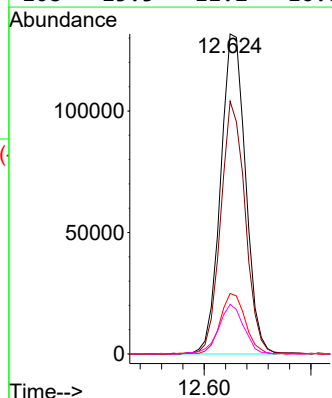





#40
Hexachlorocyclopentadiene
Concen: 10.211 ng/ul
RT: 12.601 min Scan# 1619
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:237 Resp: 42555
Ion Ratio Lower Upper
237 100
235 54.9 51.0 76.6
272 12.7 9.7 14.5

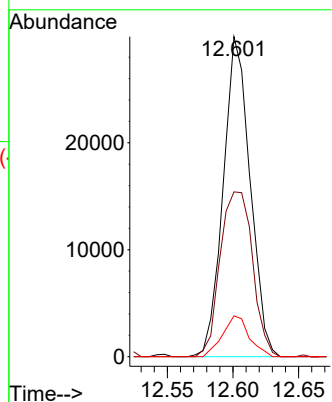

#41
2,4,6-Trichlorophenol
Concen: 21.068 ng/ul
RT: 12.877 min Scan# 1666
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:196 Resp: 125534
Ion Ratio Lower Upper
196 100
198 96.9 72.4 108.6
200 28.5 22.5 33.7


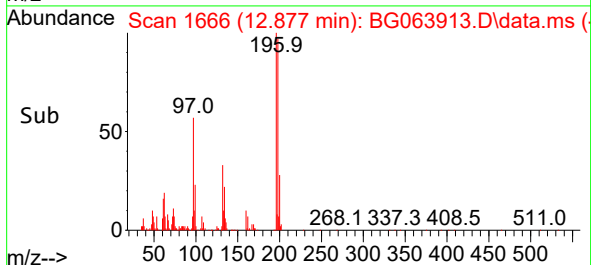






#42
2,4,5-Trichlorophenol
Concen: 21.472 ng/ul
RT: 12.953 min Scan# 1
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:196 Resp: 133524
Ion Ratio Lower Upper
196 100
198 91.3 74.2 111.4
200 33.1 23.5 35.3

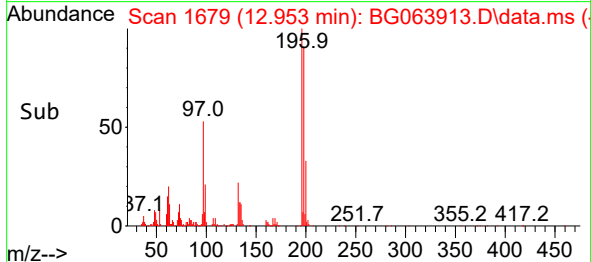

#43
1,1'-Biphenyl
Concen: 21.547 ng/ul
RT: 13.270 min Scan# 1733
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:154 Resp: 467970
Ion Ratio Lower Upper
154 100
153 40.4 35.1 52.7
76 15.9 13.4 20.2





#44

2-Chloronaphthalene

Concen: 21.286 ng/ul

RT: 13.312 min Scan# 1740

Delta R.T. 0.001 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:162 Resp: 371235

Ion Ratio Lower Upper

162 100

164 34.3 25.2 37.8

127 34.0 29.2 43.8



#45

2-Nitroaniline

Concen: 21.759 ng/ul

RT: 13.523 min Scan# 1776

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion: 65 Resp: 127109


Ion Ratio Lower Upper

65 100

92 66.1 49.5 74.3

138 81.6 61.8 92.8









#47
Dimethylphthalate
Concen: 21.257 ng/ul
RT: 13.893 min Scan# 1839
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:163 Resp: 477389
Ion Ratio Lower Upper
163 100
194 3.7 3.0 4.4
164 9.5 8.8 13.2



#48
2,6-Dinitrotoluene
Concen: 23.457 ng/ul
RT: 14.023 min Scan# 1861
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:165 Resp: 97837
Ion Ratio Lower Upper
165 100
89 63.5 59.4 89.2
121 19.0 20.8 31.2#

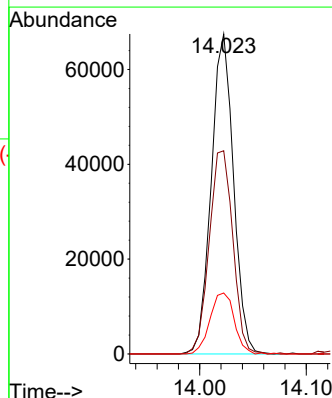



#50

Acenaphthylene

Concen: 21.805 ng/ul

RT: 14.164 min Scan# 1885

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:152 Resp: 597255

Ion Ratio Lower Upper

152 100

151 18.6 14.6 22.0

153 12.5 10.0 15.0

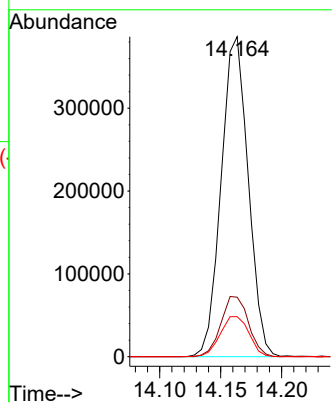

#51

3-Nitroaniline

Concen: 20.905 ng/ul

RT: 14.352 min Scan# 1917

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:138 Resp: 80615


Ion Ratio Lower Upper

138 100

108 9.9 8.4 12.6

92 126.8 120.4 180.6




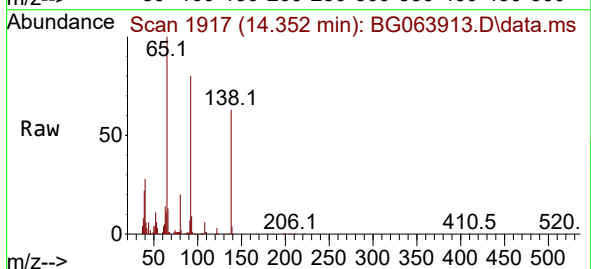




#52
Acenaphthene
Concen: 21.641 ng/ul
RT: 14.504 min Scan# 1943
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:153 Resp: 420127
Ion Ratio Lower Upper
153 100
152 46.1 40.2 60.4
154 84.7 70.8 106.2

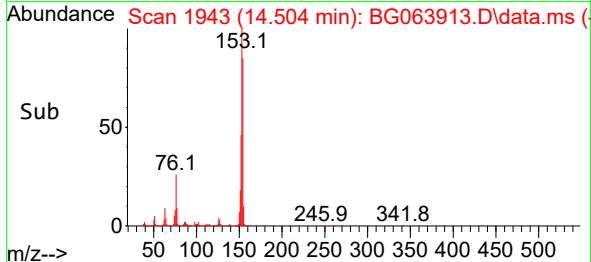

#53
2,4-Dinitrophenol
Concen: 9.390 ng/ul
RT: 14.587 min Scan# 1957
Delta R.T. 0.013 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:184 Resp: 20016
Ion Ratio Lower Upper
184 100
63 78.0 52.1 78.1
154 65.1 47.8 71.6




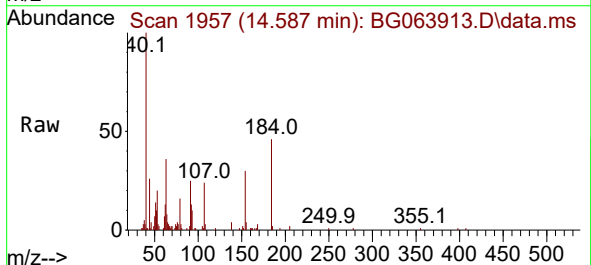




#55
4-Nitrophenol
Concen: 16.562 ng/ul
RT: 14.686 min Scan# 1974
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:109 Resp: 54604
Ion Ratio Lower Upper
109 100
139 117.7 86.4 129.6
65 153.8 127.0 190.4

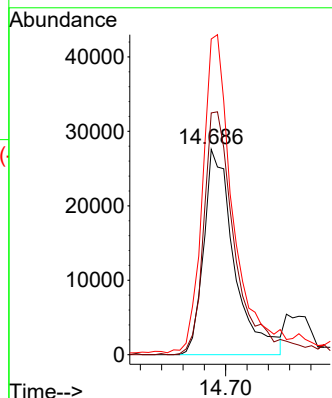

#56
Dibenzofuran
Concen: 21.832 ng/ul
RT: 14.845 min Scan# 2001
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:168 Resp: 597556
Ion Ratio Lower Upper
168 100
139 31.2 27.8 41.8



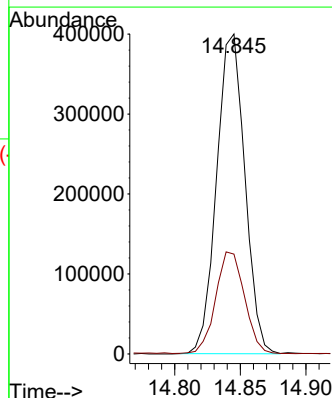





#57
2,4-Dinitrotoluene
Concen: 23.862 ng/ul
RT: 14.822 min Scan# 1996
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:165 Resp: 147887
Ion Ratio Lower Upper
165 100
63 50.6 45.0 67.4
182 2.5 1.8 2.8

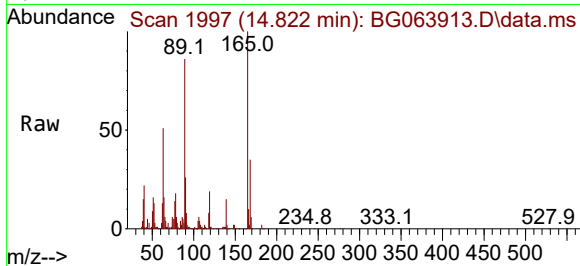

#58
2,3,4,6-Tetrachlorophenol
Concen: 21.032 ng/ul
RT: 15.080 min Scan# 2041
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:232 Resp: 112738
Ion Ratio Lower Upper
232 100
131 38.4 30.3 45.5
130 2.0 1.8 2.6
166 25.0 24.9 37.3




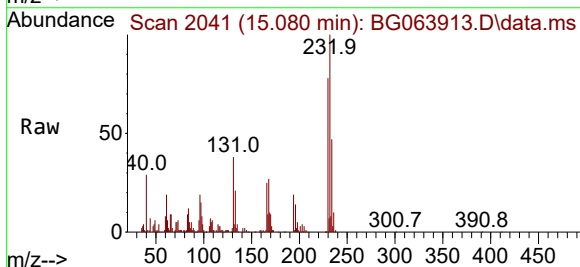




#59
Diethylphthalate
Concen: 21.795 ng/ul
RT: 15.268 min Scan# 2072
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:149 Resp: 473196
Ion Ratio Lower Upper
149 100
177 22.8 17.6 26.4
150 11.4 9.0 13.4



#61
Fluorene
Concen: 22.041 ng/ul
RT: 15.497 min Scan# 2112
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:166 Resp: 481709
Ion Ratio Lower Upper
166 100
165 101.8 81.9 122.9
167 14.2 11.4 17.0









#62
4-Chlorophenyl-phenylether
Concen: 21.220 ng/ul
RT: 15.486 min Scan# 2110
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:204 Resp: 258370
Ion Ratio Lower Upper
204 100
206 32.2 25.6 38.4
141 46.8 42.3 63.5

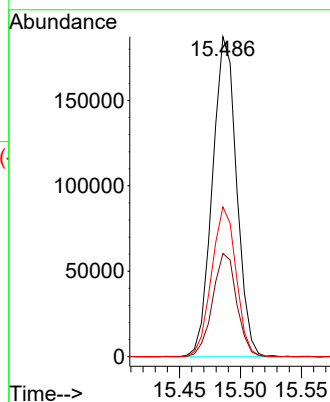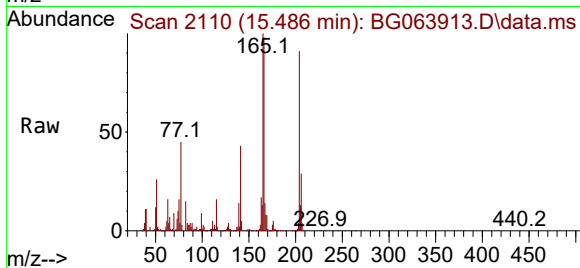

#63
4-Nitroaniline
Concen: 18.033 ng/ul
RT: 15.521 min Scan# 2116
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:138 Resp: 69621
Ion Ratio Lower Upper
138 100
92 64.7 53.2 79.8
108 86.3 79.4 119.0


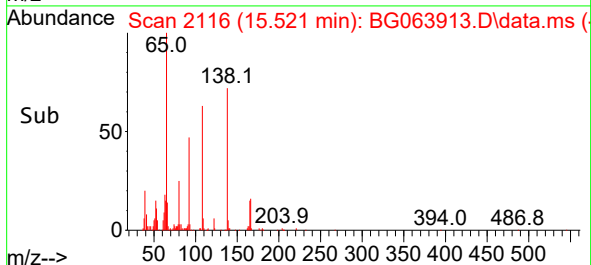

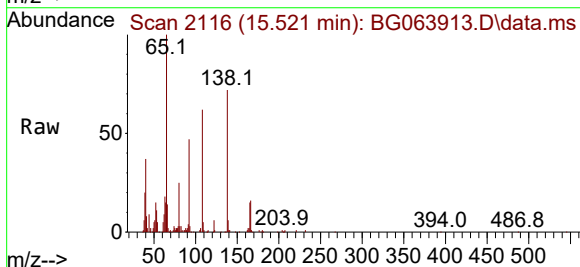




#66
 4,6-Dinitro-2-methylphenol
 Concen: 16.759 ng/ul
 RT: 15.591 min Scan# 2128
 Delta R.T. 0.007 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020589


Tgt Ion:198 Resp: 71139
 Ion Ratio Lower Upper
 198 100
 182 4.2 3.4 5.2
 77 24.2 25.2 37.8#

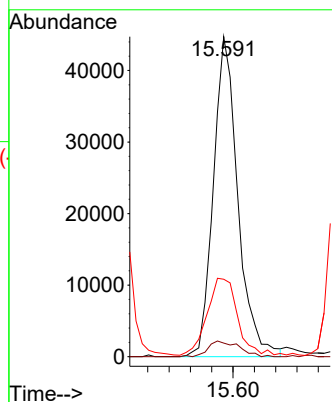

#67
 N-Nitrosodiphenylamine
 Concen: 21.948 ng/ul
 RT: 15.703 min Scan# 2147
 Delta R.T. 0.007 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38

Tgt Ion:169 Resp: 421763
 Ion Ratio Lower Upper
 169 100
 168 68.4 54.0 81.0
 167 37.7 29.8 44.8


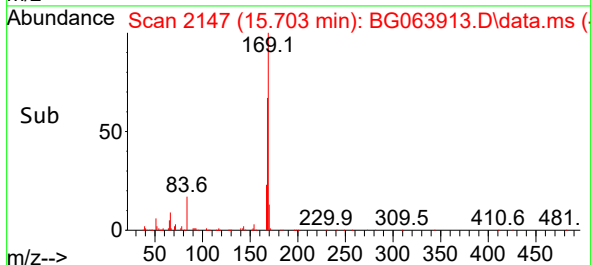






#68
4-Bromophenyl-phenylether
Concen: 21.457 ng/ul
RT: 16.384 min Scan# 21
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:248 Resp: 173535
Ion Ratio Lower Upper
248 100
250 96.7 76.1 114.1
141 56.7 46.0 69.0

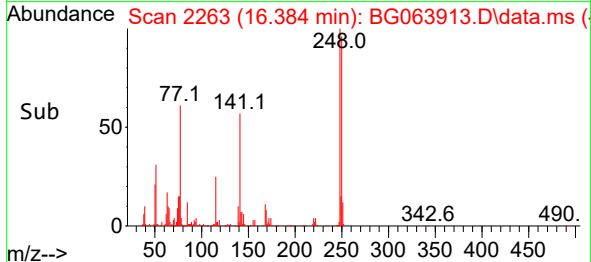

#69
Hexachlorobenzene
Concen: 21.481 ng/ul
RT: 16.508 min Scan# 2284
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:284 Resp: 194644
Ion Ratio Lower Upper
284 100
142 29.5 23.9 35.9
249 31.6 24.6 36.8





#70

Atrazine

Concen: 21.589 ng/ul

RT: 16.661 min Scan# 21

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:200 Resp: 175372

Ion Ratio Lower Upper

200 100

173 22.5 21.3 31.9

215 48.1 37.8 56.8



#71

Pentachlorophenol

Concen: 13.517 ng/ul

RT: 16.866 min Scan# 2345

Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:266 Resp: 51640


Ion Ratio Lower Upper

266 100

264 56.6 49.3 73.9

268 54.9 50.5 75.7


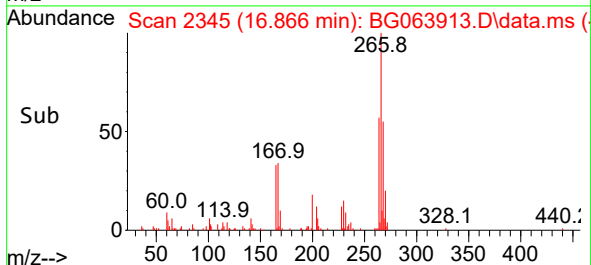
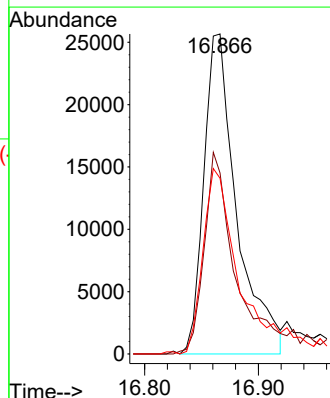





#72
Phenanthrene
Concen: 22.552 ng/ul
RT: 17.236 min Scan# 2408
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:178 Resp: 862424
Ion Ratio Lower Upper
178 100
179 15.4 12.2 18.2
176 19.2 15.8 23.6



#74
Anthracene
Concen: 22.594 ng/ul
RT: 17.330 min Scan# 2424
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:178 Resp: 874539
Ion Ratio Lower Upper
178 100
179 15.1 12.4 18.6
176 17.6 14.4 21.6









#75
1,2,3,4-Tetrachlorobenzene
Concen: 20.217 ng/ul
RT: 13.235 min Scan# 1727
Delta R.T. 0.001 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:216 Resp: 214051
Ion Ratio Lower Upper
216 100
214 79.3 60.2 90.4
218 46.4 37.6 56.4

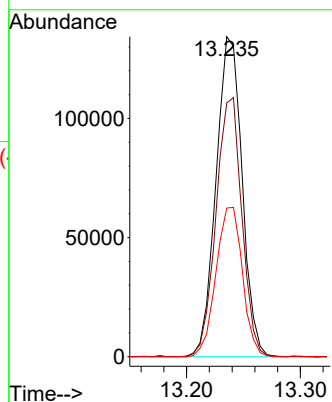

#76
Pentachlorobenzene
Concen: 21.144 ng/ul
RT: 14.769 min Scan# 1988
Delta R.T. 0.007 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:250 Resp: 221780
Ion Ratio Lower Upper
250 100
248 60.3 49.8 74.8
252 64.1 50.4 75.6









#77
 Carbazole
 Concen: 23.586 ng/ul
 RT: 17.607 min Scan# 2471
 Delta R.T. 0.013 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020589


Tgt Ion:167 Resp: 738984
 Ion Ratio Lower Upper
 167 100
 166 22.3 18.2 27.4
 139 11.1 10.1 15.1



#78
 Di-n-butylphthalate
 Concen: 23.487 ng/ul
 RT: 18.165 min Scan# 2566
 Delta R.T. 0.013 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38

Tgt Ion:149 Resp: 888705
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.2 10.8
 104 5.4 5.4 8.0





#80

Fluoranthene

Concen: 21.604 ng/ul

RT: 19.263 min Scan# 21

Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:202 Resp: 1020278

Ion Ratio Lower Upper

202 100

101 10.5 8.1 12.1

100 8.2 6.5 9.7



#82

Pyrene

Concen: 22.017 ng/ul

RT: 19.628 min Scan# 2815

Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:202 Resp: 1106258


Ion Ratio Lower Upper

202 100

101 12.1 8.7 13.1

100 10.6 7.8 11.6

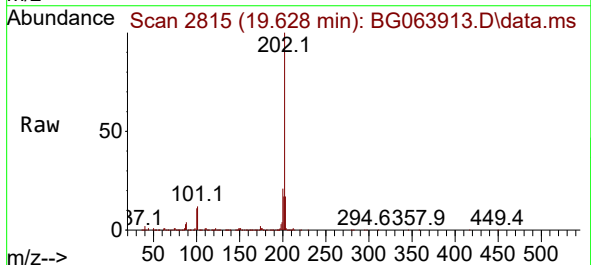



#83

Butylbenzylphthalate

Concen: 23.150 ng/ul

RT: 20.521 min Scan# 2967

Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:149 Resp: 357063

Ion Ratio Lower Upper

149 100

91 84.9 68.7 103.1

206 23.2 17.3 25.9



#84

3,3'-Dichlorobenzidine

Concen: 20.899 ng/ul

RT: 21.349 min Scan# 3108

Delta R.T. 0.007 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:252 Resp: 301235


Ion Ratio Lower Upper

252 100

254 62.1 55.8 83.6

126 8.5 6.4 9.6









#85
Benzo(a)anthracene
Concen: 20.909 ng/ul
RT: 21.432 min Scan# 3122
Delta R.T. 0.013 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38




Instrument :
BNA_G
ClientSampleId :
SSTD020589


Tgt Ion:228 Resp: 1046298
Ion Ratio Lower Upper
228 100
229 19.9 15.7 23.5
226 27.0 22.0 33.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 24.365 ng/ul
RT: 21.343 min Scan# 3107
Delta R.T. 0.013 min
Lab File: BG063913.D
Acq: 28 Dec 2024 21:38

Tgt Ion:149 Resp: 546663
Ion Ratio Lower Upper
149 100
167 27.0 22.1 33.1
279 3.8 2.9 4.3





#87

Chrysene

Concen: 20.744 ng/ul

RT: 21.496 min Scan# 3132

Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:228 Resp: 989372

Ion Ratio Lower Upper

228 100

226 29.4 23.4 35.0

229 18.9 14.8 22.2



#89

Di-n-octyl phthalate

Concen: 25.430 ng/ul




RT: 22.477 min Scan# 3300


Delta R.T. 0.013 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Tgt Ion:149 Resp: 898860





#90

Benzo(b)fluoranthene

Concen: 21.646 ng/ul

RT: 23.517 min Scan# 3476

Delta R.T. 0.018 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:252 Resp: 1007473

Ion Ratio Lower Upper

252 100

253 21.0 17.7 26.5

125 9.3 7.0 10.4

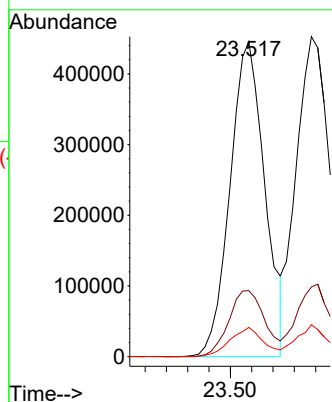

#91

Benzo(k)fluoranthene

Concen: 21.700 ng/ul

RT: 23.517 min Scan# 3477

Delta R.T. -0.040 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:252 Resp: 1007473


Ion Ratio Lower Upper

252 100

253 21.0 17.7 26.5

125 9.3 6.5 9.7





#93

Benzo(a)pyrene

Concen: 21.400 ng/ul

RT: 24.328 min Scan# 3

Delta R.T. 0.024 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38

Instrument :

BNA_G

ClientSampleId :

SSTD020589





Tgt Ion:252 Resp: 934887

Ion Ratio Lower Upper

252 100

253 22.4 16.6 24.8

125 9.7 8.0 12.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 22.202 ng/ul

RT: 27.871 min Scan# 4218

Delta R.T. 0.024 min

Lab File: BG063913.D

Acq: 28 Dec 2024 21:38




Tgt Ion:276 Resp: 1184514


Ion Ratio Lower Upper

276 100

138 17.4 13.7 20.5

277 23.0 18.4 27.6

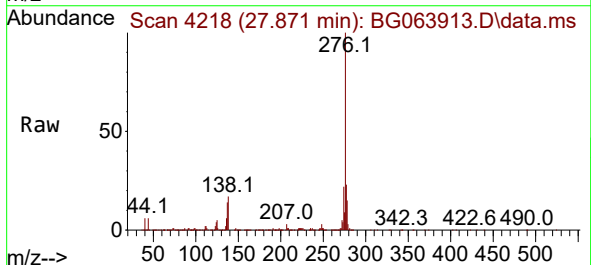




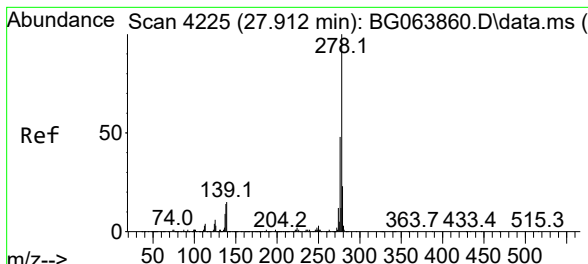


#95
 Dibenzo(a,h)anthracene
 Concen: 22.011 ng/ul
 RT: 27.930 min Scan# 41
 Delta R.T. 0.042 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020589

Tgt Ion:278 Resp: 939672

Ion	Ratio	Lower	Upper
278	100		
139	13.1	9.7	14.5
279	25.0	17.3	25.9

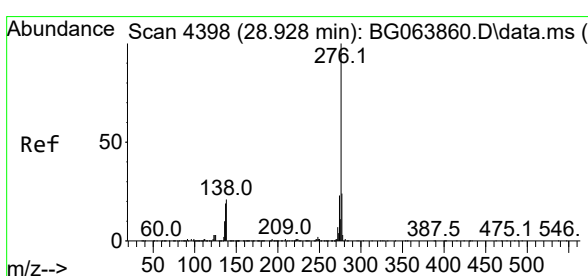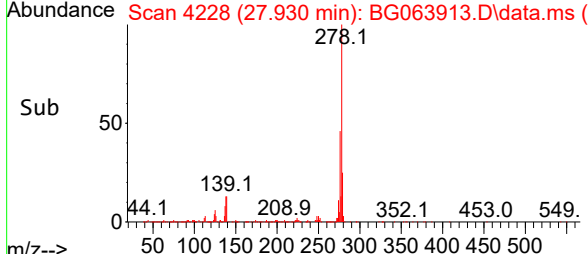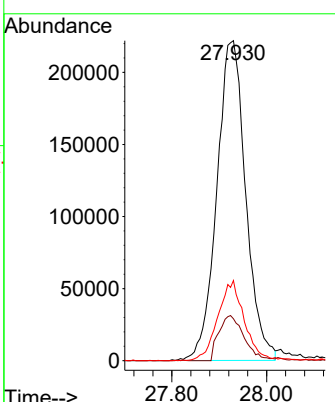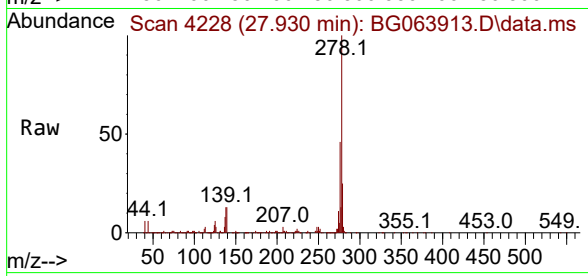

#96
 Benzo(g,h,i)perylene
 Concen: 21.829 ng/ul
 RT: 28.946 min Scan# 4401
 Delta R.T. 0.048 min
 Lab File: BG063913.D
 Acq: 28 Dec 2024 21:38

Tgt Ion:276 Resp: 924159

Ion	Ratio	Lower	Upper
276	100		
138	19.9	13.8	20.8
277	24.5	17.8	26.8

