




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

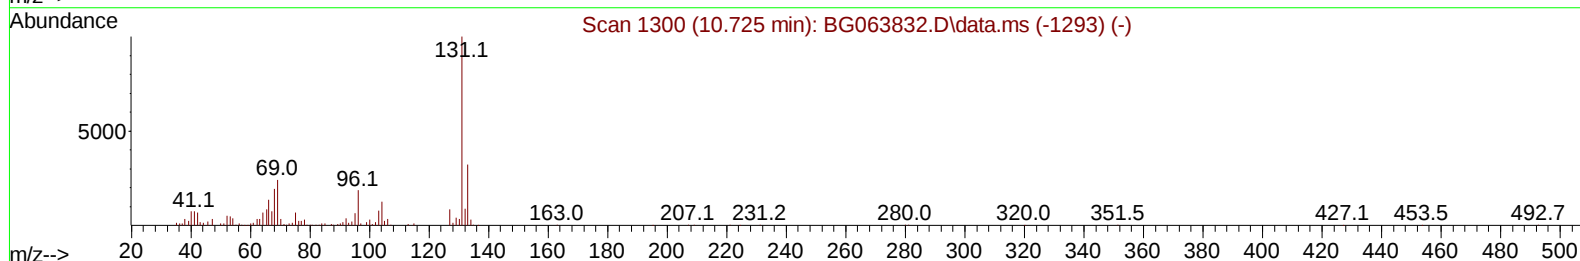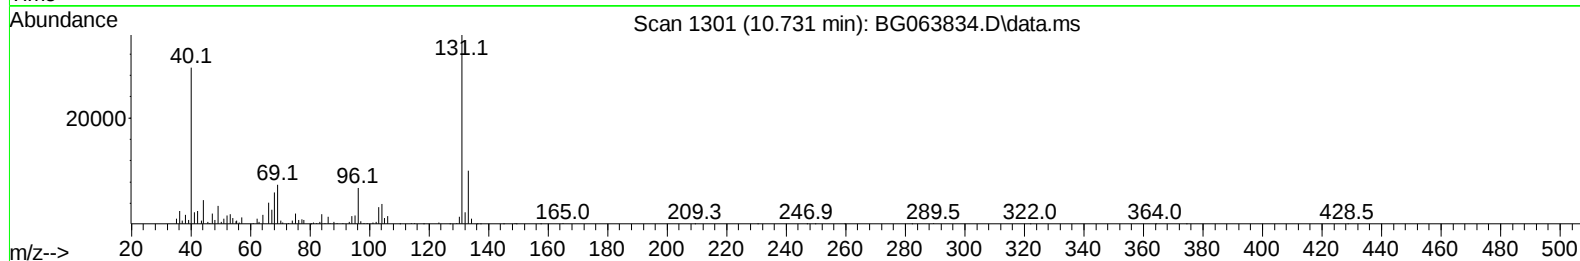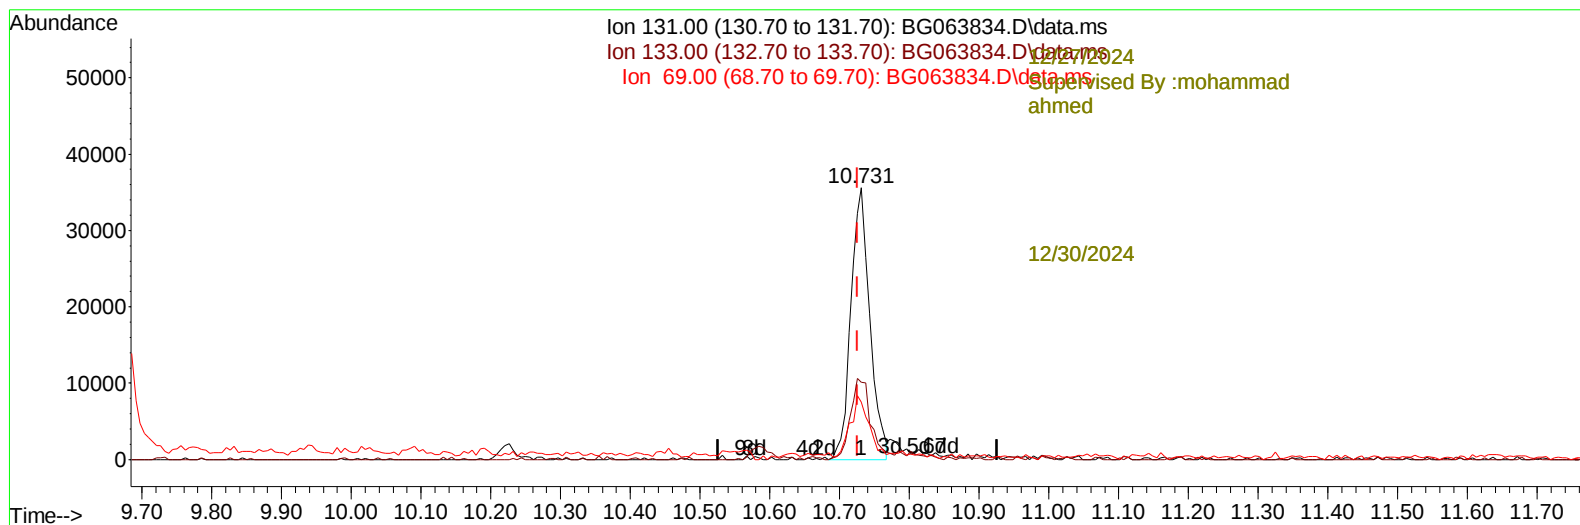

TIC: BG063834.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.731min (+ 0.006) 10.65 ng/u1

response 67107

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.30	28.53
69.00	23.80	21.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

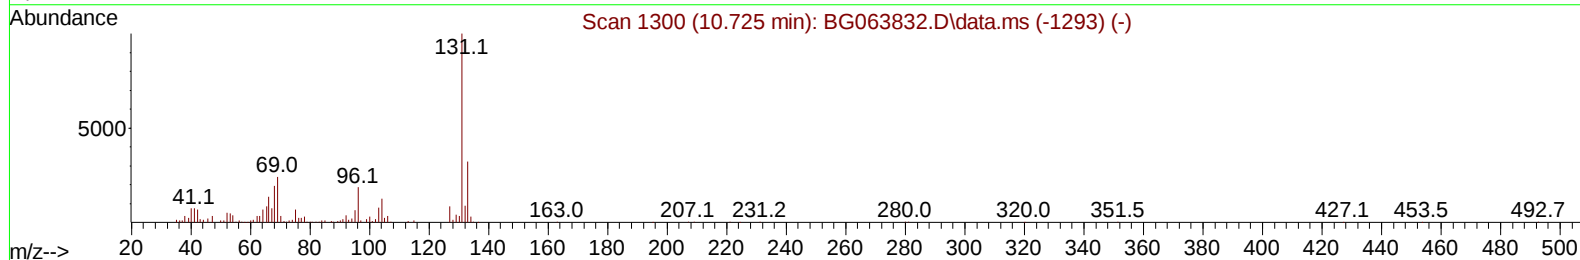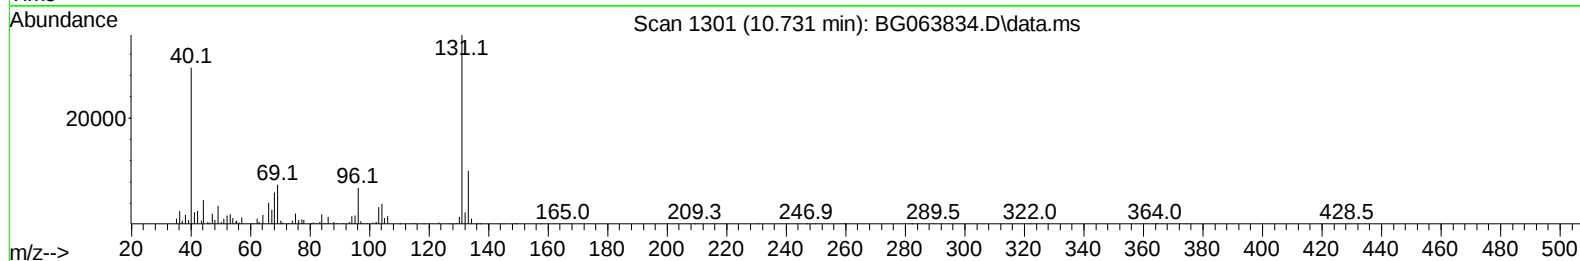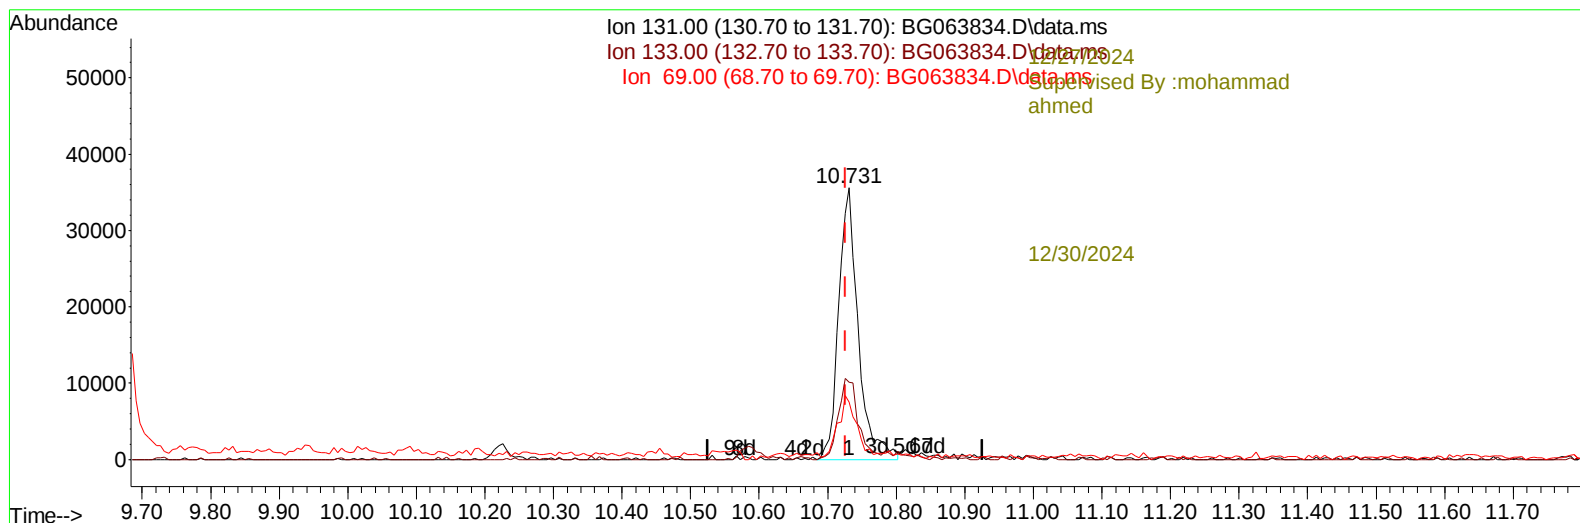

TIC: BG063834.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.731min (+ 0.006) 11.21 ng/ul m

response 70673

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.30	28.53
69.00	23.80	21.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

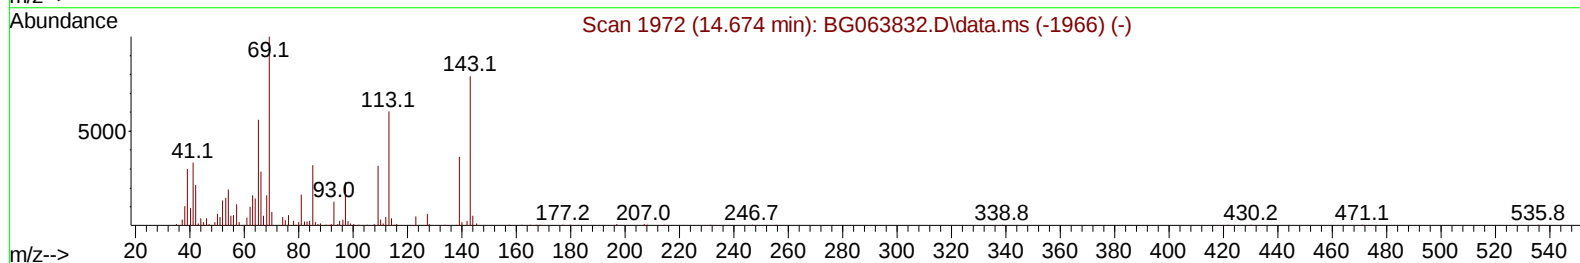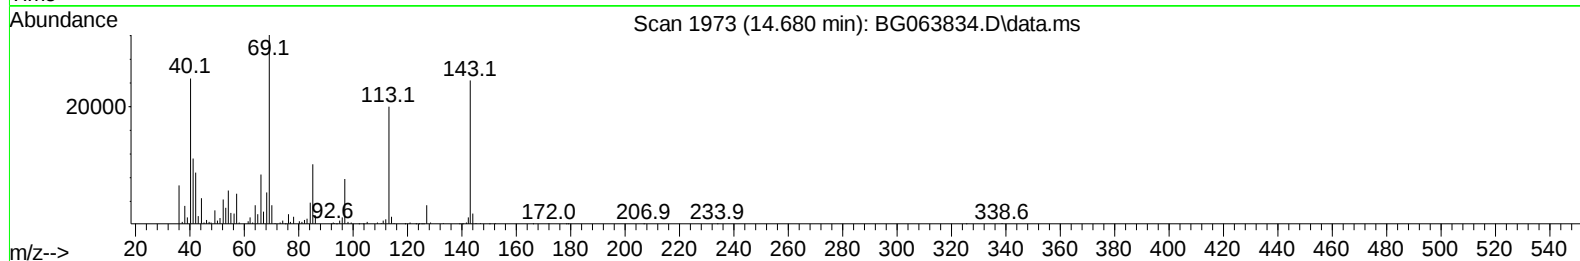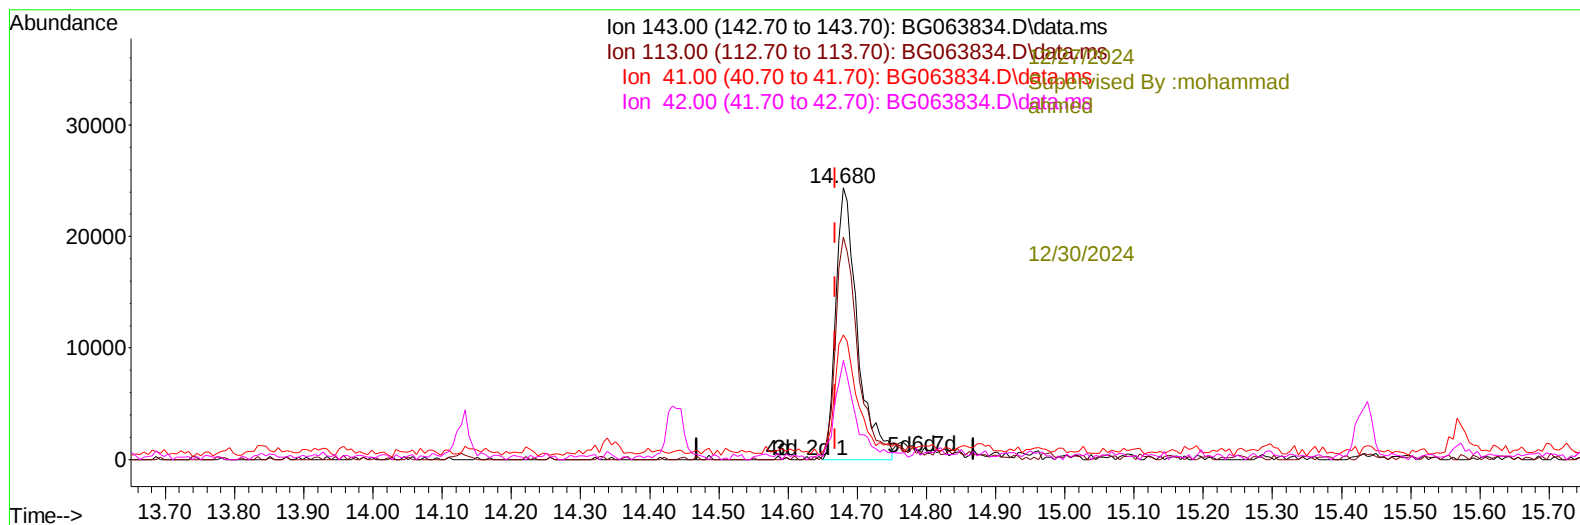

TIC: BG063834.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.680min (+ 0.012) 20.73 ng/u1

response 52800

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	82.00
41.00	48.20	45.98
42.00	26.60	36.34#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

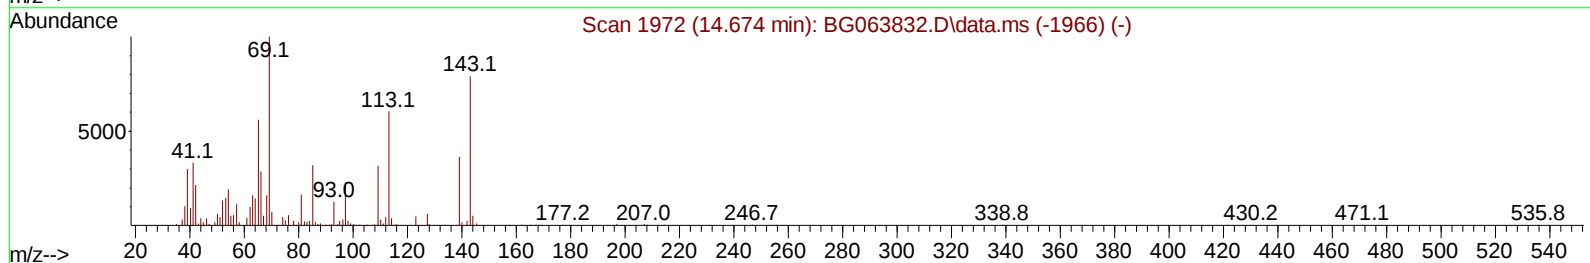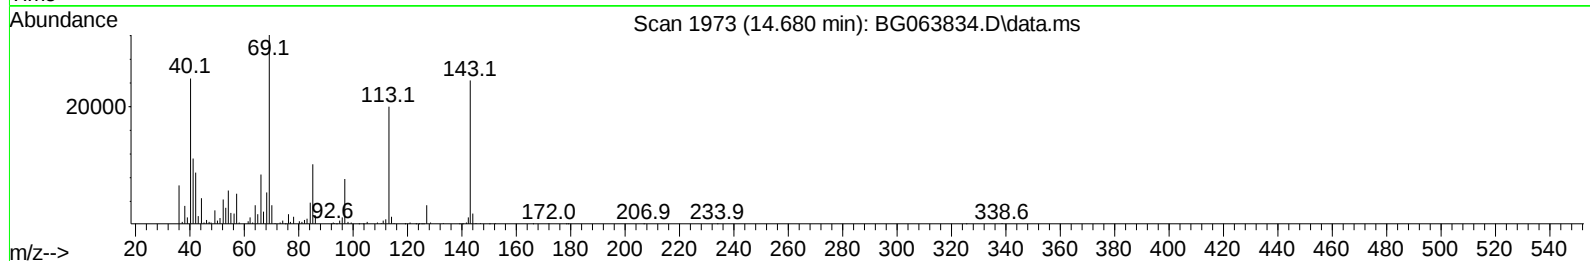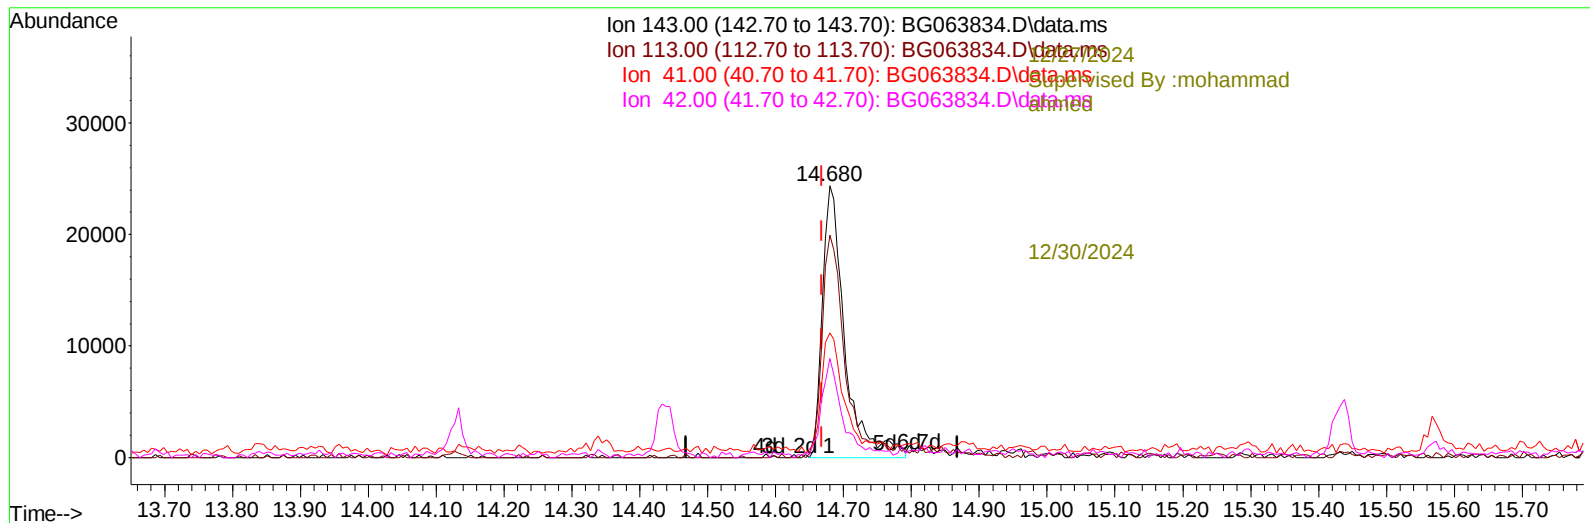

TIC: BG063834.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.680min (+ 0.012) 21.82 ng/ul m

response 55579

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	82.00
41.00	48.20	45.98
42.00	26.60	36.34#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 02:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

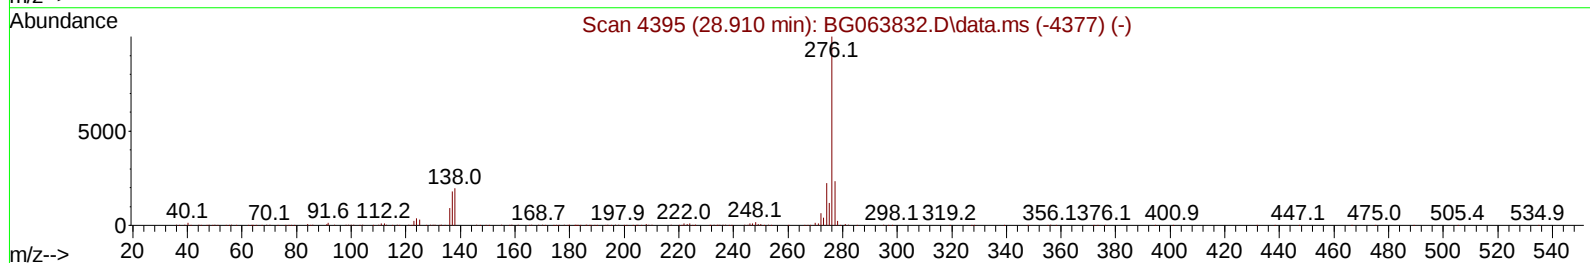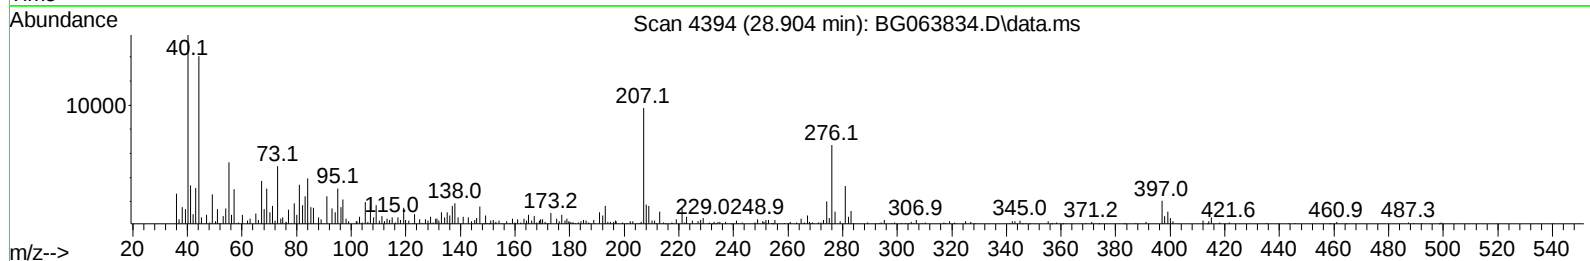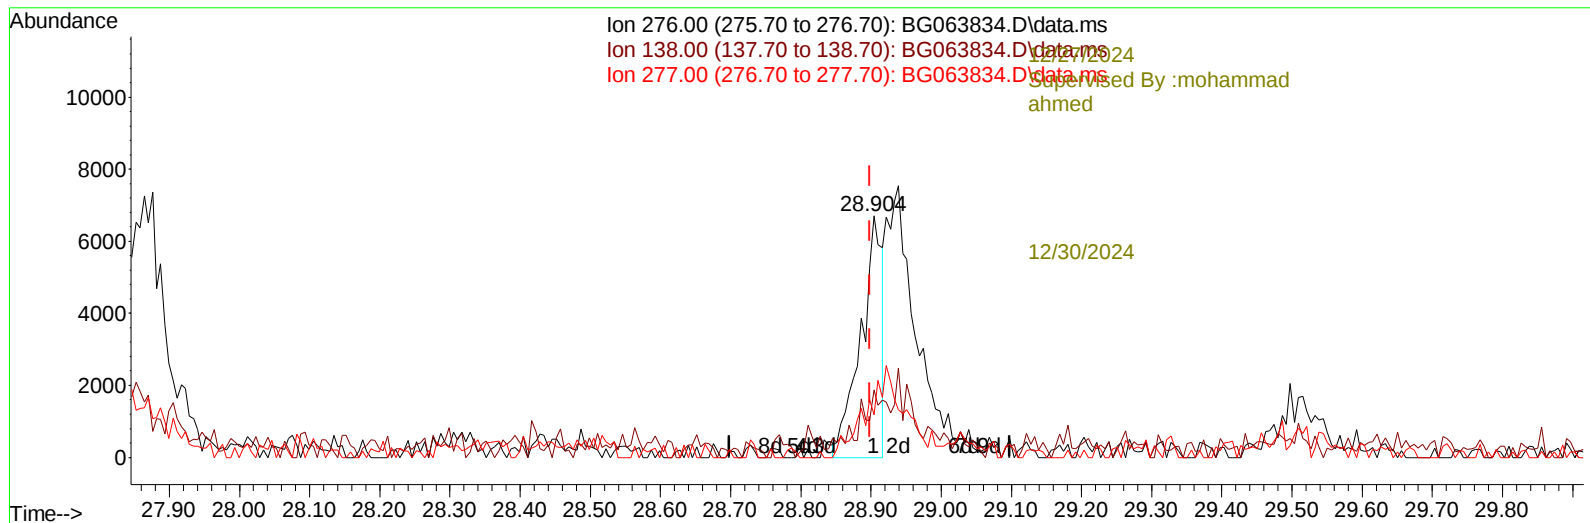

TIC: BG063834.D\data.ms

(96) Benzo(g,h,i)perylene

28.904min (+ 0.006) 0.42 ng/uL

response 14071

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	28.00#
277.00	22.30	17.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 02:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

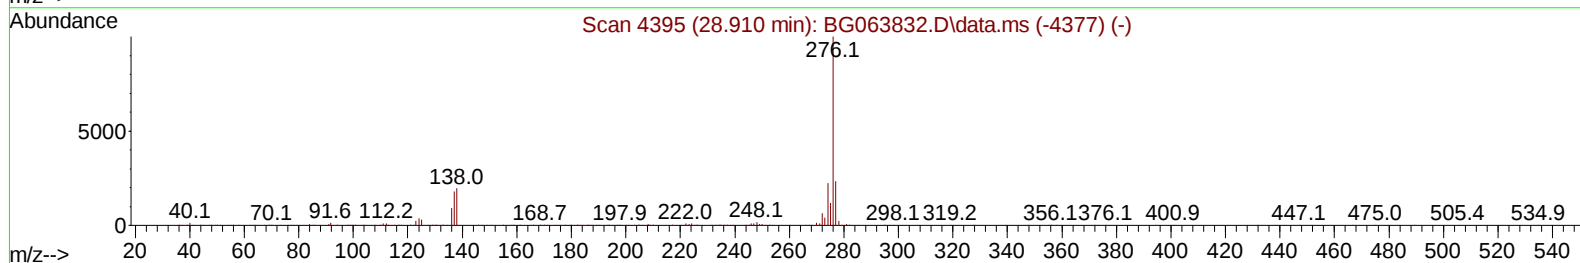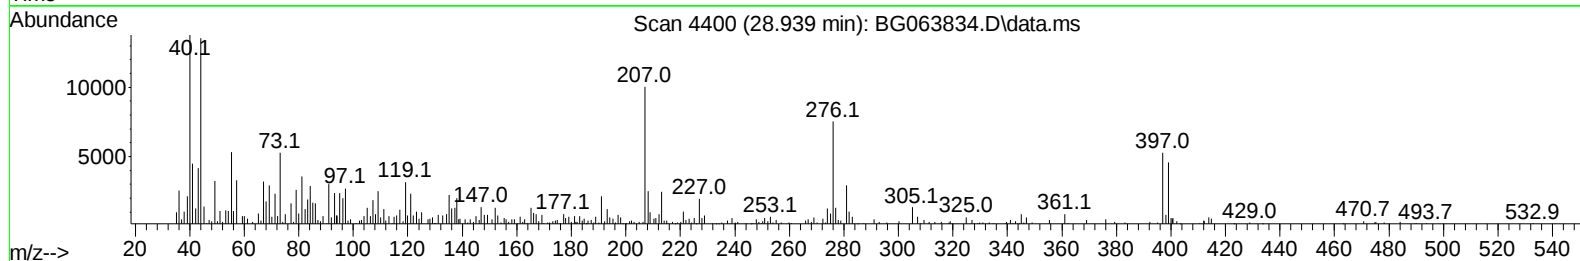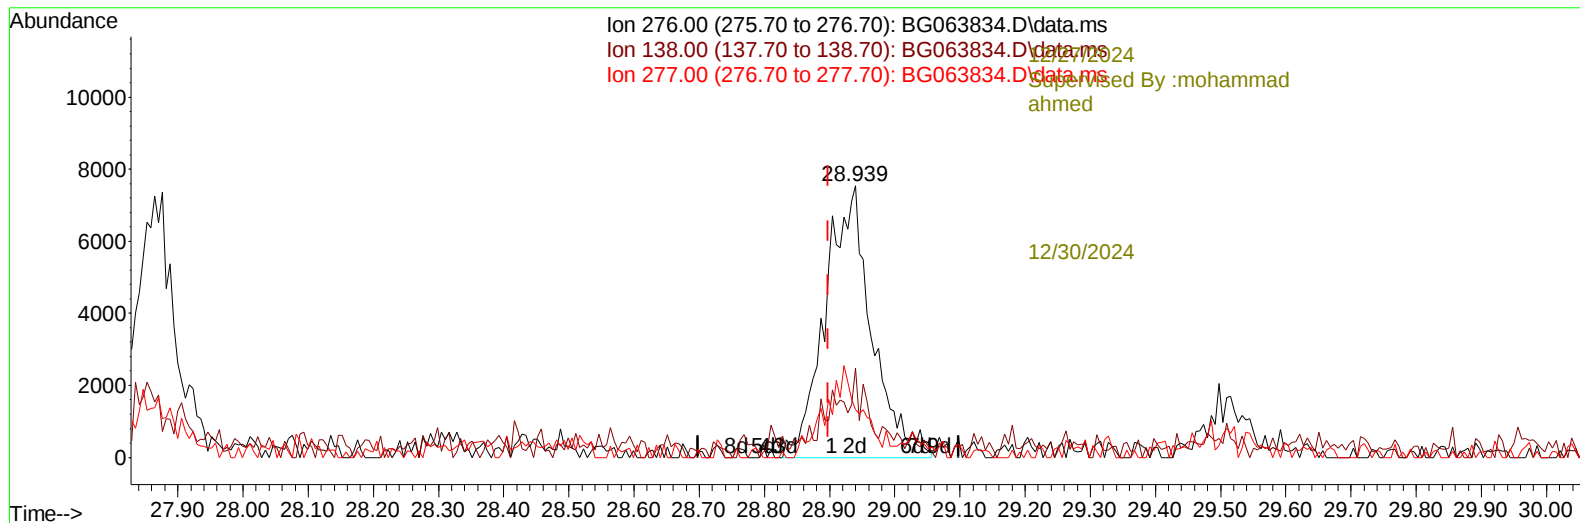

TIC: BG063834.D\data.ms

(96) Benzo(g,h,i)perylene

28.939min (+ 0.041) 1.11 ng/ul m

response 37090

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	26.72#
277.00	22.30	17.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063834.D
 Acq On : 26 Dec 2024 14:31
 Operator : RC/JU
 Sample : P5333-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 02:10:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 00:44:39 2024
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----12/27/2024							
Supervised By :mohammad ali med							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.794	152		69154	20.000	ng/ul	0.00
20) Naphthalene-d8	10.584	136		320327	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164		264239	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.188	188		614715	20.000	ng/ul	0.00
79) Chrysene-d12	21.442	240		610610	20.000	ng/ul	0.00
88) Perylene-d12	24.456	264		648024	20.000	ng/ul	0.00
-----12/30/2024							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.252	96		10450	5.922	ng/uL	0.00
4) Pyridine-d5	3.663	84		136730	24.561	ng/ul	0.00
7) Phenol-d5	6.983	99		158520	24.889	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.130	67		100659	22.883	ng/ul	0.00
11) 2-Chlorophenol-d4	7.335	132		103496	25.100	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113		121035	24.477	ng/ul	0.00
21) Nitrobenzene-d5	8.951	128		55545	24.286	ng/ul	0.00
24) 2-Nitrophenol-d4	9.674	143		64513	25.163	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.226	165		117737	23.719	ng/ul	0.00
31) 4-Chloroaniline-d4	10.731	131		70673m	11.213	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166		433811	24.127	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160		442199	21.574	ng/ul	0.00
54) 4-Nitrophenol-d4	14.680	143		55579m	21.817	ng/ul	0.01
60) Fluorene-d10	15.438	176		310841	19.553	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.573	200		56326	17.648	ng/ul	0.00
73) Anthracene-d10	17.288	188		513594	19.433	ng/ul	0.00
81) Pyrene-d10	19.592	212		513377	16.157	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.251	264		419948	13.800	ng/ul	0.00
Target Compounds							
						Qvalue	
8) Phenol	7.012	94		8367	1.233	ng/ul#	86
72) Phenanthrene	17.235	178		53430	1.804	ng/ul#	92
80) Fluoranthene	19.257	202		96768	2.679	ng/ul#	95
82) Pyrene	19.621	202		87777	2.284	ng/ul#	88
85) Benzo(a)anthracene	21.419	228		45625	1.192	ng/ul	98
87) Chrysene	21.483	228		43105	1.182	ng/ul	95
90) Benzo(b)fluoranthene	23.516	252		54271	1.474	ng/ul#	92
93) Benzo(a)pyrene	24.315	252		40625	1.175	ng/ul#	82
96) Benzo(g,h,i)perylene	28.939	276		37090m	1.107	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063834.D
Acq On : 26 Dec 2024 14:31
Operator : RC/JU
Sample : P5333-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2911

Manual IntegrationsAPPROVED

Quant Time: Dec 27 02:10:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

