




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063841.D
Acq On : 26 Dec 2024 18:54
Operator : RC/JU
Sample : P5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YE5Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:22:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

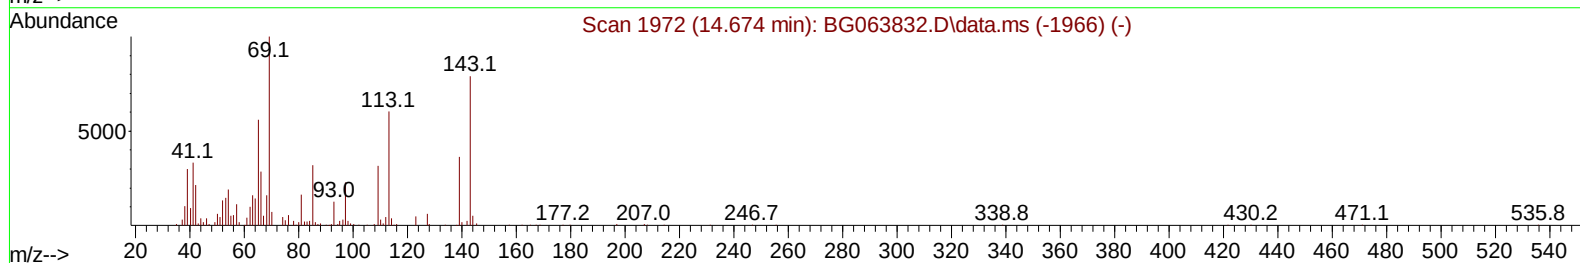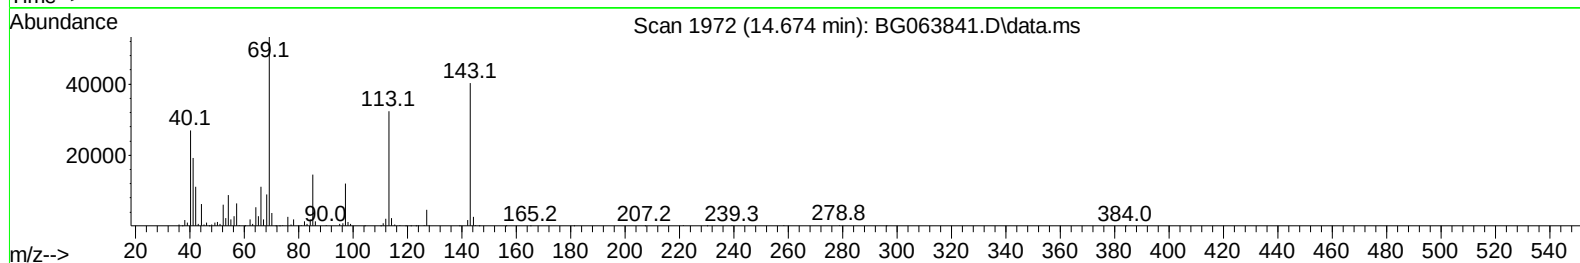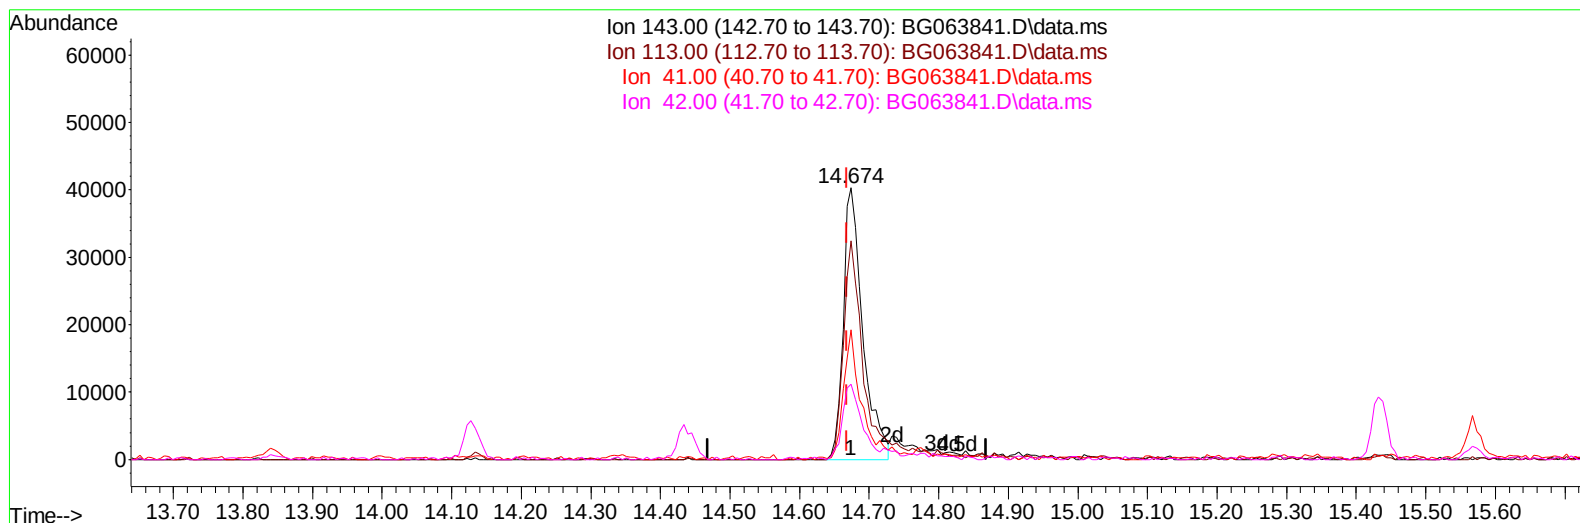

TIC: BG063841.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.674min (+ 0.006) 28.79 ng/ul

response 78308

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	80.54
41.00	48.20	47.75
42.00	26.60	27.74




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063841.D
Acq On : 26 Dec 2024 18:54
Operator : RC/JU
Sample : P5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YE5Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 01:22:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

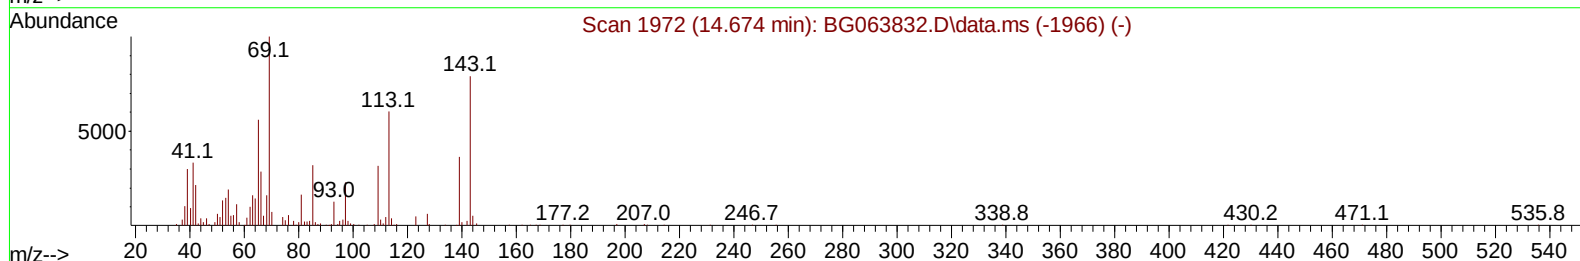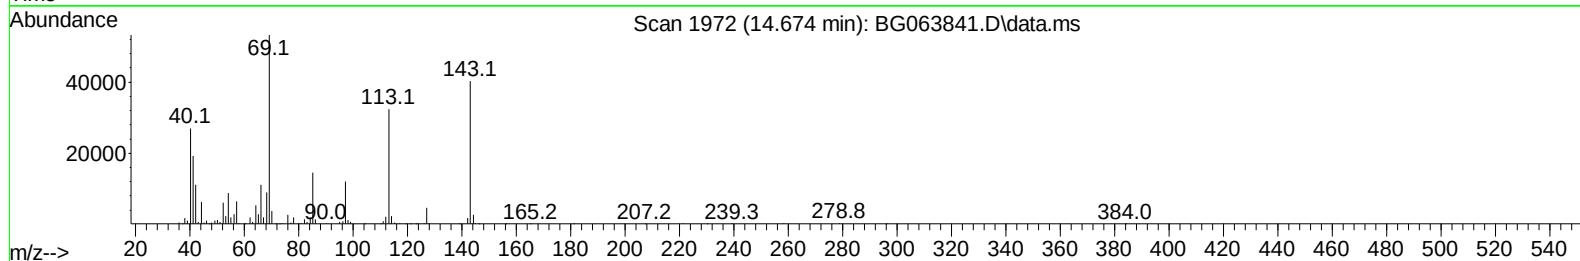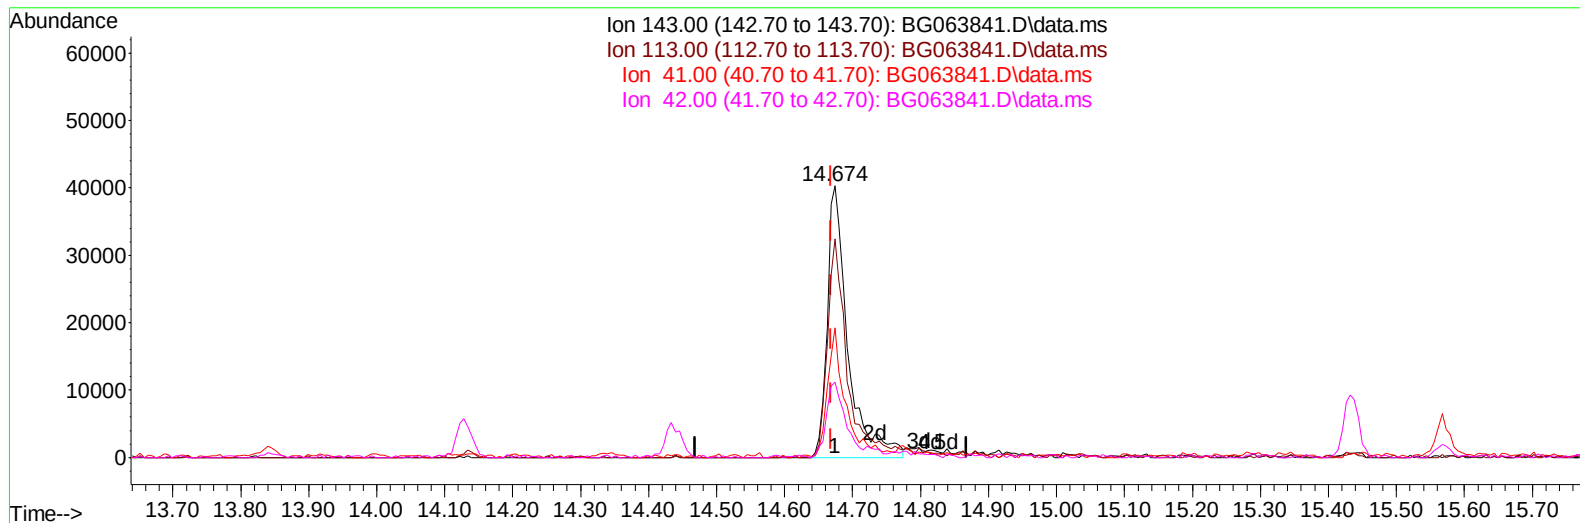

TIC: BG063841.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.674min (+ 0.006) 31.17 ng/ul m

response 84779

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	80.54
41.00	48.20	47.75
42.00	26.60	27.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063841.D
 Acq On : 26 Dec 2024 18:54
 Operator : RC/JU
 Sample : P5324-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YE5Y1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/27/2024
 Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 27 02:36:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 24 00:44:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	89056	20.000	ng/ul	0.00
20) Naphthalene-d8	10.585	136	364024	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	282085	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.189	188	692673	20.000	ng/ul	0.00
79) Chrysene-d12	21.443	240	713790	20.000	ng/ul	0.00
88) Perylene-d12	24.457	264	772812	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	10988	4.835	ng/uL	0.00
4) Pyridine-d5	3.664	84	176921	24.679	ng/ul	0.00
7) Phenol-d5	6.983	99	214957	26.208	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.124	67	142297	25.119	ng/ul	0.00
11) 2-Chlorophenol-d4	7.336	132	138154	26.018	ng/ul	0.00
15) 4-Methylphenol-d8	8.517	113	163100	25.613	ng/ul	0.00
21) Nitrobenzene-d5	8.952	128	78483	30.196	ng/ul	0.00
24) 2-Nitrophenol-d4	9.674	143	94329	32.376	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.221	165	162204	28.755	ng/ul	0.00
31) 4-Chloroaniline-d4	10.726	131	221640	30.945	ng/ul	0.00
46) Dimethylphthalate-d6	13.846	166	614746	32.027	ng/ul	0.00
49) Acenaphthylene-d8	14.128	160	703556	32.154	ng/ul	0.00
54) 4-Nitrophenol-d4	14.674	143	84779m	31.173	ng/ul	0.00
60) Fluorene-d10	15.432	176	568129	33.477	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.573	200	82989	23.076	ng/ul	0.00
73) Anthracene-d10	17.289	188	1038049	34.857	ng/ul	0.00
81) Pyrene-d10	19.592	212	1217197	32.770	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.251	264	1166406	32.140	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063841.D
Acq On : 26 Dec 2024 18:54
Operator : RC/JU
Sample : P5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YE5Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 02:36:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 24 00:44:39 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

