

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063893.D
 Acq On : 28 Dec 2024 7:50
 Operator : RC/JU
 Sample : PB165892BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.668	94	99	115	rBV	364686	702753	22.66%	2.459%
2	6.988	657	664	674	rBV	433672	760709	24.53%	2.661%
3	7.129	683	688	697	rVB	353965	585928	18.89%	2.050%
4	7.335	717	723	734	rVB	437504	747923	24.12%	2.617%
5	7.799	796	802	809	rVB	311807	537886	17.34%	1.882%
6	8.516	918	924	935	rBV2	526557	911952	29.41%	3.191%
7	8.786	968	970	971	rBV2	7342	5349	0.17%	0.019%
8	8.950	992	998	1005	rBV	400190	696157	22.45%	2.436%
9	9.279	1052	1054	1056	rBV	5890	4904	0.16%	0.017%
10	9.356	1065	1067	1070	rBV	5551	6370	0.21%	0.022%
11	9.561	1100	1102	1105	rVB	7194	6192	0.20%	0.022%
12	9.673	1114	1121	1128	rBV2	330221	573712	18.50%	2.007%
13	9.949	1167	1168	1169	rBV	8046	5108	0.16%	0.018%
14	10.220	1208	1214	1224	rBV	456543	861686	27.79%	3.015%
15	10.584	1269	1276	1283	rBV	395758	712999	22.99%	2.495%
16	10.725	1293	1300	1318	rVB	421023	823279	26.55%	2.880%
17	10.995	1345	1346	1348	rBV	6888	4866	0.16%	0.017%
18	11.201	1379	1381	1383	rVB	7775	4822	0.16%	0.017%
19	11.306	1397	1399	1404	rVB2	4916	6591	0.21%	0.023%
20	11.353	1404	1407	1410	rBV4	4511	7086	0.23%	0.025%
21	11.395	1410	1414	1415	rBV2	4434	4866	0.16%	0.017%
22	11.812	1484	1485	1488	rBV2	5343	5843	0.19%	0.020%
23	11.865	1492	1494	1498	rVV2	5569	7082	0.23%	0.025%
24	11.900	1498	1500	1504	rVB	5490	5580	0.18%	0.020%
25	12.188	1544	1549	1550	rBV3	9787	14896	0.48%	0.052%
26	12.529	1604	1607	1608	rBV2	6255	5827	0.19%	0.020%
27	12.769	1644	1648	1650	rVB2	6213	6107	0.20%	0.021%
28	12.840	1659	1660	1662	rBV2	5647	5128	0.17%	0.018%
29	13.122	1706	1708	1711	rVB2	4650	5072	0.16%	0.018%
30	13.157	1711	1714	1715	rBV2	6699	5964	0.19%	0.021%
31	13.257	1730	1731	1734	rVB3	5074	4567	0.15%	0.016%
32	13.286	1734	1736	1740	rBV2	5863	5935	0.19%	0.021%
33	13.422	1756	1759	1763	rBV3	4478	5529	0.18%	0.019%
34	13.804	1822	1824	1825	rBV	7159	4577	0.15%	0.016%
35	13.845	1825	1831	1841	rVB	856344	1255058	40.47%	4.391%
36	14.044	1862	1865	1868	rVB3	5887	8131	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063893.D
Acq On : 28 Dec 2024 7:50
Operator : RC/JU
Sample : PB165892BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Title : SVOA CALIBRATION

37	14.080	1868	1871	1872	rBV	7621	5187	0.17%	0.018%
38	14.133	1872	1880	1890	rBV2	1032440	1610681	51.94%	5.635%
39	14.391	1919	1924	1925	rBV2	4359	4768	0.15%	0.017%
40	14.438	1925	1932	1940	rVB	650837	1017126	32.80%	3.559%

41	14.573	1953	1955	1958	rBV	5893	5746	0.19%	0.020%
42	14.679	1967	1973	1992	rBV2	211299	532851	17.18%	1.864%
43	14.926	2012	2015	2020	rBV3	6882	11207	0.36%	0.039%
44	15.061	2036	2038	2040	rVB	6108	5175	0.17%	0.018%
45	15.120	2045	2048	2052	rBV4	3889	6504	0.21%	0.023%

46	15.208	2062	2063	2068	rVB2	5418	7422	0.24%	0.026%
47	15.337	2083	2085	2089	rBV3	3871	5470	0.18%	0.019%
48	15.437	2095	2102	2111	rBV	1324461	2009687	64.80%	7.031%
49	15.578	2120	2126	2138	rBV2	201737	365611	11.79%	1.279%
50	15.684	2141	2144	2148	rVB5	12593	18106	0.58%	0.063%

51	15.883	2176	2178	2183	rVB3	6138	8773	0.28%	0.031%
52	15.930	2183	2186	2187	rBV	4951	4551	0.15%	0.016%
53	15.966	2190	2192	2195	rBV2	4225	5320	0.17%	0.019%
54	16.083	2210	2212	2213	rBV	5926	5043	0.16%	0.018%
55	16.130	2219	2220	2224	rVB2	4707	5281	0.17%	0.018%

56	16.171	2224	2227	2230	rBV2	6976	6093	0.20%	0.021%
57	16.212	2231	2234	2236	rVB	4933	4866	0.16%	0.017%
58	16.477	2277	2279	2282	rVB2	5265	4679	0.15%	0.016%
59	16.735	2321	2323	2326	rBV2	6423	6206	0.20%	0.022%
60	16.829	2335	2339	2342	rBV3	5763	6699	0.22%	0.023%

61	16.912	2351	2353	2355	rBV	4462	4641	0.15%	0.016%
62	16.982	2360	2365	2369	rVB3	5520	9094	0.29%	0.032%
63	17.076	2380	2381	2384	rBV2	6050	4689	0.15%	0.016%
64	17.141	2390	2392	2394	rVB3	6303	5537	0.18%	0.019%
65	17.194	2394	2401	2408	rBV	934253	1388268	44.77%	4.857%

66	17.294	2411	2418	2428	rVV	1590756	2424719	78.19%	8.483%
67	17.382	2431	2433	2435	rVV	6366	5613	0.18%	0.020%
68	17.405	2435	2437	2440	rVB	9704	9415	0.30%	0.033%
69	17.440	2440	2443	2444	rBV3	5460	5438	0.18%	0.019%
70	17.464	2444	2447	2449	rBV2	3413	4649	0.15%	0.016%

71	17.564	2461	2464	2467	rBV3	5815	6857	0.22%	0.024%
72	17.816	2504	2507	2509	rBV4	6097	7264	0.23%	0.025%
73	17.858	2511	2514	2516	rVV3	9185	10160	0.33%	0.036%
74	17.875	2516	2517	2521	rVB3	5505	5284	0.17%	0.018%
75	18.234	2576	2578	2583	rVV2	6199	7679	0.25%	0.027%

76	18.281	2583	2586	2587	rVB2	6500	5045	0.16%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063893.D
 Acq On : 28 Dec 2024 7:50
 Operator : RC/JU
 Sample : PB165892BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

77	18.339	2593	2596	2598	rVB	5819	5506	0.18%	0.019%
78	18.433	2609	2612	2615	rBV2	4372	6009	0.19%	0.021%
79	18.480	2618	2620	2622	rBV2	4510	4512	0.15%	0.016%
80	18.657	2648	2650	2652	rBV2	4824	4549	0.15%	0.016%
81	18.686	2652	2655	2656	rVB3	7407	6438	0.21%	0.023%
82	18.868	2684	2686	2689	rBV2	4951	4740	0.15%	0.017%
83	18.892	2689	2690	2693	rBV	6099	5823	0.19%	0.020%
84	19.080	2718	2722	2725	rBV3	5865	8862	0.29%	0.031%
85	19.103	2725	2726	2729	rBV3	4948	5225	0.17%	0.018%
86	19.156	2729	2735	2740	rVV5	28002	43745	1.41%	0.153%
87	19.232	2745	2748	2754	rVV2	25979	34851	1.12%	0.122%
88	19.285	2756	2757	2759	rVB2	8445	4890	0.16%	0.017%
89	19.309	2759	2761	2764	rBV3	5623	7268	0.23%	0.025%
90	19.373	2771	2772	2775	rBV2	8109	8768	0.28%	0.031%
91	19.403	2775	2777	2779	rVV	3689	4505	0.15%	0.016%
92	19.462	2785	2787	2788	rBV2	6454	4429	0.14%	0.015%
93	19.520	2794	2797	2800	rBV3	6475	9435	0.30%	0.033%
94	19.597	2803	2810	2821	rBV	2174649	3101217	100.00%	10.850%
95	19.920	2861	2865	2866	rBV4	5406	6107	0.20%	0.021%
96	20.073	2889	2891	2893	rBV3	5393	5578	0.18%	0.020%
97	20.343	2935	2937	2938	rBV2	7700	6402	0.21%	0.022%
98	21.448	3119	3125	3141	rBV2	1027434	1742591	56.19%	6.097%
99	24.262	3594	3604	3617	rBV	1104214	2967155	95.68%	10.381%
100	24.468	3631	3639	3651	rVB	622269	1700078	54.82%	5.948%




Sum of corrected areas: 28582521

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063893.D
Acq On : 28 Dec 2024 7:50
Operator : RC/JU
Sample : PB165892BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

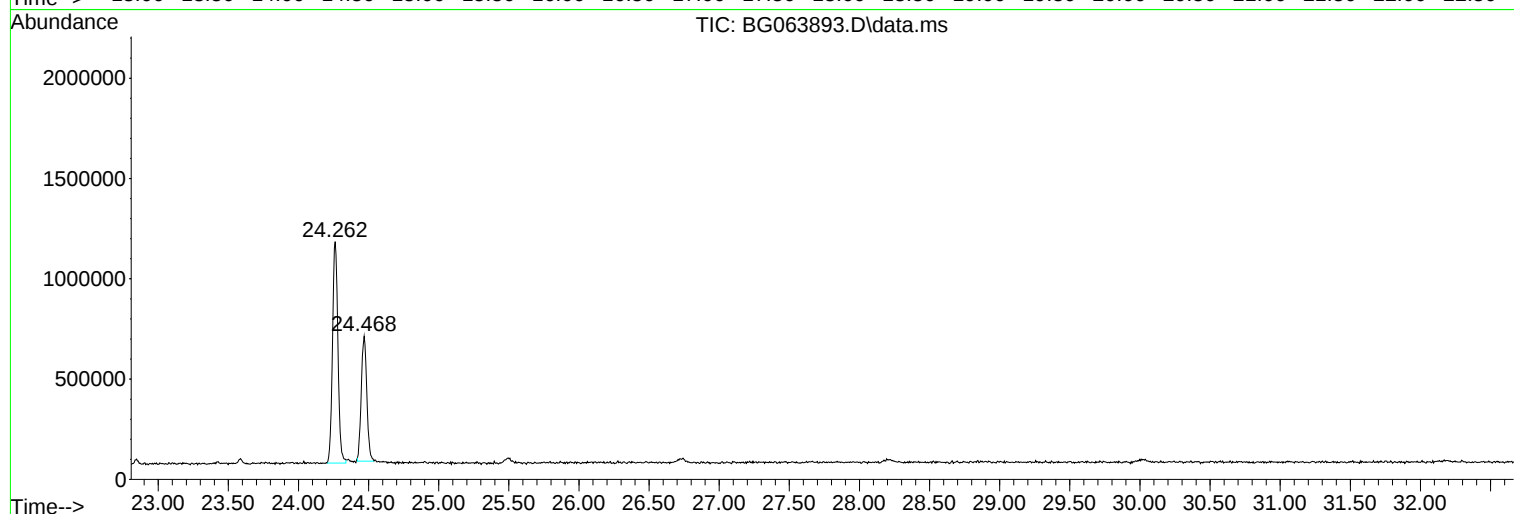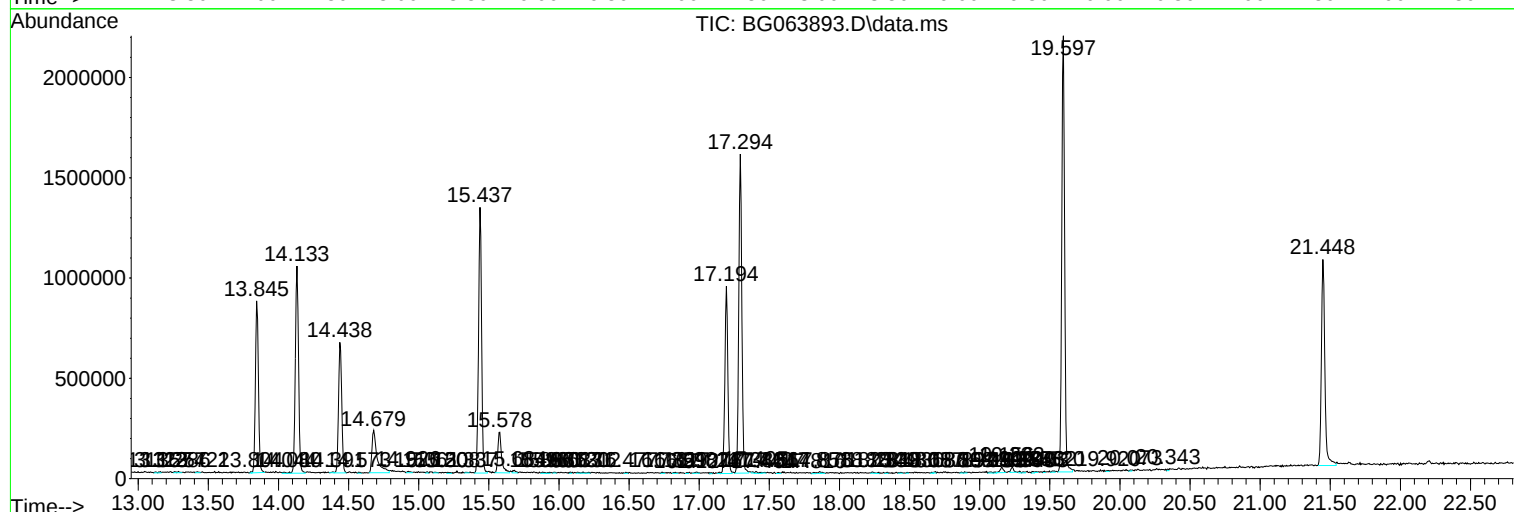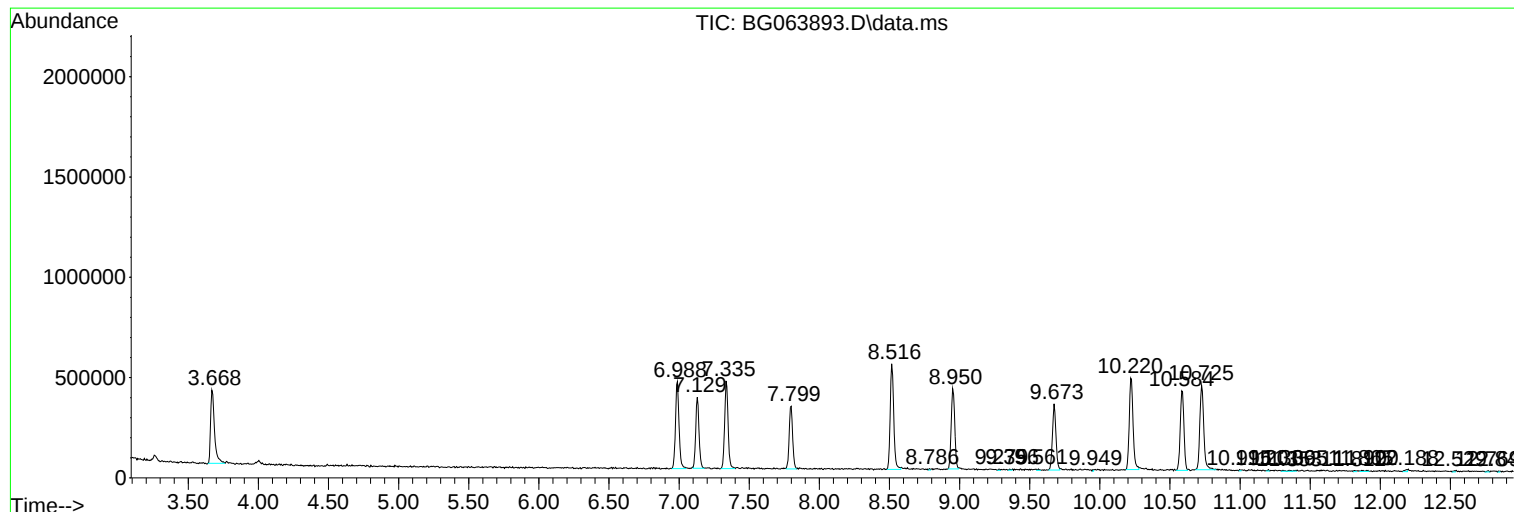

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063893.D
Acq On : 28 Dec 2024 7:50
Operator : RC/JU
Sample : PB165892BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063893.D
Acq On : 28 Dec 2024 7:50
Operator : RC/JU
Sample : PB165892BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc