

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063906.D
 Acq On : 28 Dec 2024 16:37
 Operator : RC/JU
 Sample : PB165893BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK893

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.667	94	98	114	rBV	480764	814810	23.77%	2.453%
2	6.698	612	614	616	rBV2	8540	7860	0.23%	0.024%
3	6.986	656	663	672	rBV	538115	907241	26.47%	2.731%
4	7.127	682	687	699	rVB	401236	671325	19.59%	2.021%
5	7.339	716	723	730	rBV	516839	871045	25.41%	2.622%
6	7.797	795	801	811	rVB	345356	563329	16.44%	1.696%
7	8.520	917	924	936	rBV	641343	1118571	32.64%	3.368%
8	8.955	990	998	1007	rBV	464204	846752	24.70%	2.549%
9	9.225	1042	1044	1046	rBV	5120	5358	0.16%	0.016%
10	9.677	1113	1121	1130	rBV	383774	705913	20.60%	2.125%
11	9.977	1170	1172	1174	rBV	7741	5974	0.17%	0.018%
12	10.141	1197	1200	1201	rBV	7341	7343	0.21%	0.022%
13	10.224	1206	1214	1230	rBV	607307	1151459	33.59%	3.467%
14	10.588	1269	1276	1286	rVB	453887	822264	23.99%	2.476%
15	10.729	1292	1300	1312	rBV	528019	1044777	30.48%	3.146%
16	10.923	1331	1333	1334	rBV	7765	6557	0.19%	0.020%
17	11.076	1356	1359	1361	rBV2	4292	5673	0.17%	0.017%
18	11.228	1384	1385	1390	rBV2	4532	6045	0.18%	0.018%
19	11.557	1439	1441	1443	rVB	7328	5836	0.17%	0.018%
20	11.816	1482	1485	1487	rBV2	4722	6018	0.18%	0.018%
21	11.916	1500	1502	1505	rVB2	4733	4577	0.13%	0.014%
22	11.957	1505	1509	1510	rBV2	4773	5129	0.15%	0.015%
23	12.022	1518	1520	1523	rBV2	4807	5652	0.16%	0.017%
24	12.174	1544	1546	1547	rBV2	7436	6127	0.18%	0.018%
25	12.721	1636	1639	1641	rBV2	5490	6391	0.19%	0.019%
26	12.785	1645	1650	1657	rBV2	6840	18305	0.53%	0.055%
27	12.903	1668	1670	1672	rVB2	6173	5704	0.17%	0.017%
28	12.921	1672	1673	1675	rBV	6136	5659	0.17%	0.017%
29	13.103	1700	1704	1706	rVB2	5710	7465	0.22%	0.022%
30	13.150	1710	1712	1718	rVB3	6996	8559	0.25%	0.026%
31	13.849	1824	1831	1839	rBV	1065258	1582327	46.17%	4.764%
32	13.949	1846	1848	1851	rBV2	4544	4808	0.14%	0.014%
33	14.078	1867	1870	1873	rBV	4843	7446	0.22%	0.022%
34	14.131	1873	1879	1890	rVV	1252273	2035749	59.39%	6.129%
35	14.266	1900	1902	1905	rVB	6196	5701	0.17%	0.017%
36	14.442	1925	1932	1940	rBV	805775	1244736	36.32%	3.748%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
 Data File : BG063906.D
 Acq On : 28 Dec 2024 16:37
 Operator : RC/JU
 Sample : PB165893BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK893

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

37	14.577	1951	1955	1959	rVB2	5518	9452	0.28%	0.028%
38	14.619	1959	1962	1965	rVB2	3743	5387	0.16%	0.016%
39	14.683	1965	1973	1984	rBV	261329	597240	17.43%	1.798%
40	15.048	2032	2035	2039	rBV4	5554	8017	0.23%	0.024%
41	15.194	2058	2060	2062	rBV	7669	4957	0.14%	0.015%
42	15.353	2084	2087	2090	rVB3	4834	5862	0.17%	0.018%
43	15.441	2095	2102	2109	rBV	1672117	2518418	73.48%	7.582%
44	15.576	2120	2125	2134	rBV	255804	431459	12.59%	1.299%
45	15.729	2149	2151	2155	rVB	4871	5773	0.17%	0.017%
46	15.758	2155	2156	2160	rBV2	5403	5053	0.15%	0.015%
47	15.964	2189	2191	2194	rVB2	4188	4651	0.14%	0.014%
48	16.111	2213	2216	2219	rBV	4073	4966	0.14%	0.015%
49	16.317	2249	2251	2254	rBV2	5738	5855	0.17%	0.018%
50	16.446	2269	2273	2274	rBV2	3335	5034	0.15%	0.015%
51	16.458	2274	2275	2281	rVB2	4558	5839	0.17%	0.018%
52	16.546	2288	2290	2292	rVB	6544	5443	0.16%	0.016%
53	16.575	2292	2295	2296	rBV	5477	4779	0.14%	0.014%
54	16.599	2296	2299	2301	rBV2	6806	5836	0.17%	0.018%
55	16.981	2361	2364	2367	rBV2	6642	6873	0.20%	0.021%
56	17.151	2390	2393	2394	rBV	9529	7547	0.22%	0.023%
57	17.198	2394	2401	2409	rVV2	1065242	1623895	47.38%	4.889%
58	17.298	2411	2418	2432	rVV2	1925856	2967792	86.59%	8.935%
59	17.603	2467	2470	2471	rVB	5808	4957	0.14%	0.015%
60	17.627	2471	2474	2476	rBV	5514	6352	0.19%	0.019%
61	17.897	2515	2520	2521	rVB4	4483	6526	0.19%	0.020%
62	17.962	2526	2531	2532	rBV2	4099	6436	0.19%	0.019%
63	18.162	2560	2565	2569	rBV3	6279	14448	0.42%	0.043%
64	18.391	2603	2604	2606	rBV	7511	6184	0.18%	0.019%
65	18.438	2610	2612	2614	rBV2	6056	5365	0.16%	0.016%
66	18.508	2621	2624	2626	rVB3	4375	4513	0.13%	0.014%
67	18.596	2636	2639	2642	rBV4	5879	6113	0.18%	0.018%
68	18.743	2662	2664	2667	rBV4	5803	5839	0.17%	0.018%
69	18.767	2667	2668	2671	rBV2	6946	6812	0.20%	0.021%
70	19.078	2720	2721	2722	rBV	7646	4752	0.14%	0.014%
71	19.154	2731	2734	2741	rVB6	28756	47889	1.40%	0.144%
72	19.231	2743	2747	2752	rVV3	26472	42271	1.23%	0.127%
73	19.278	2754	2755	2759	rBV3	5739	5731	0.17%	0.017%
74	19.319	2759	2762	2764	rVB2	7464	6868	0.20%	0.021%
75	19.337	2764	2765	2767	rBV	6349	4753	0.14%	0.014%
76	19.525	2794	2797	2800	rBV3	7422	10310	0.30%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063906.D
Acq On : 28 Dec 2024 16:37
Operator : RC/JU
Sample : PB165893BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK893

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Title : SVOA CALIBRATION

77	19.595	2803	2809	2822	rVV	2320633	3427477	100.00%	10.319%
78	19.836	2848	2850	2852	rBV2	6603	6570	0.19%	0.020%
79	19.918	2862	2864	2866	rBV3	6762	6521	0.19%	0.020%
80	20.006	2877	2879	2881	rBV3	7167	4709	0.14%	0.014%
81	20.406	2946	2947	2949	rBV2	9614	5387	0.16%	0.016%
82	21.452	3118	3125	3142	rBV2	1047390	1822501	53.17%	5.487%
83	24.266	3594	3604	3617	rBV	1194684	3179524	92.77%	9.573%
84	24.472	3631	3639	3651	rVB2	683842	1797497	52.44%	5.412%




Sum of corrected areas: 33214918

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063906.D
Acq On : 28 Dec 2024 16:37
Operator : RC/JU
Sample : PB165893BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

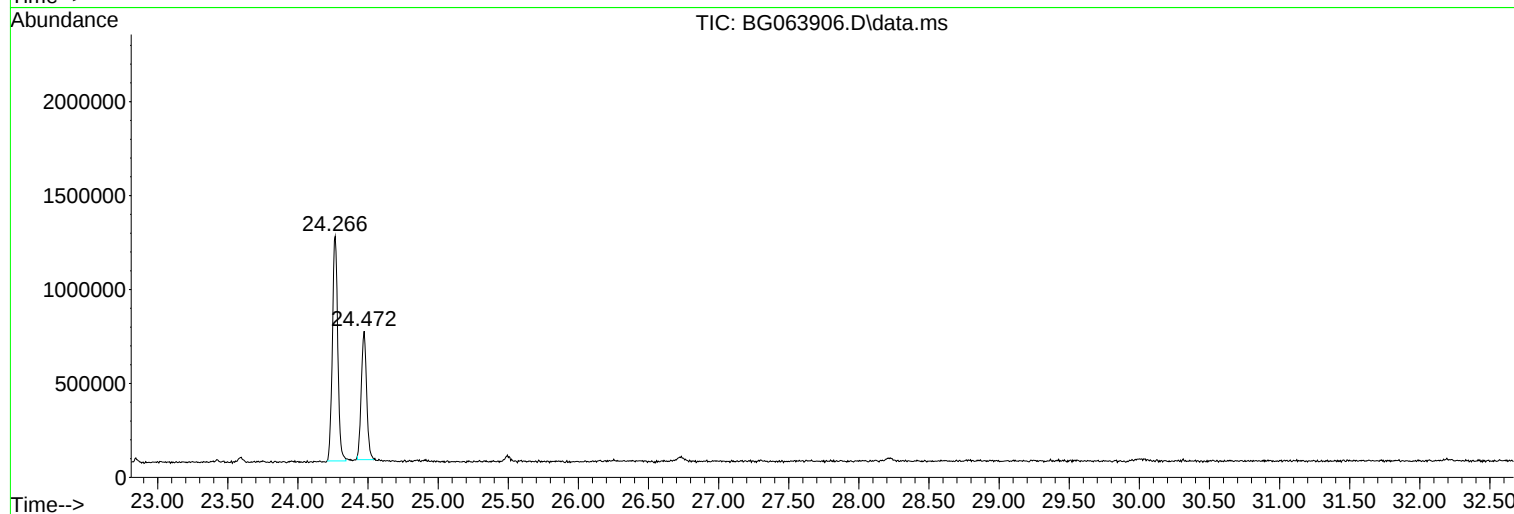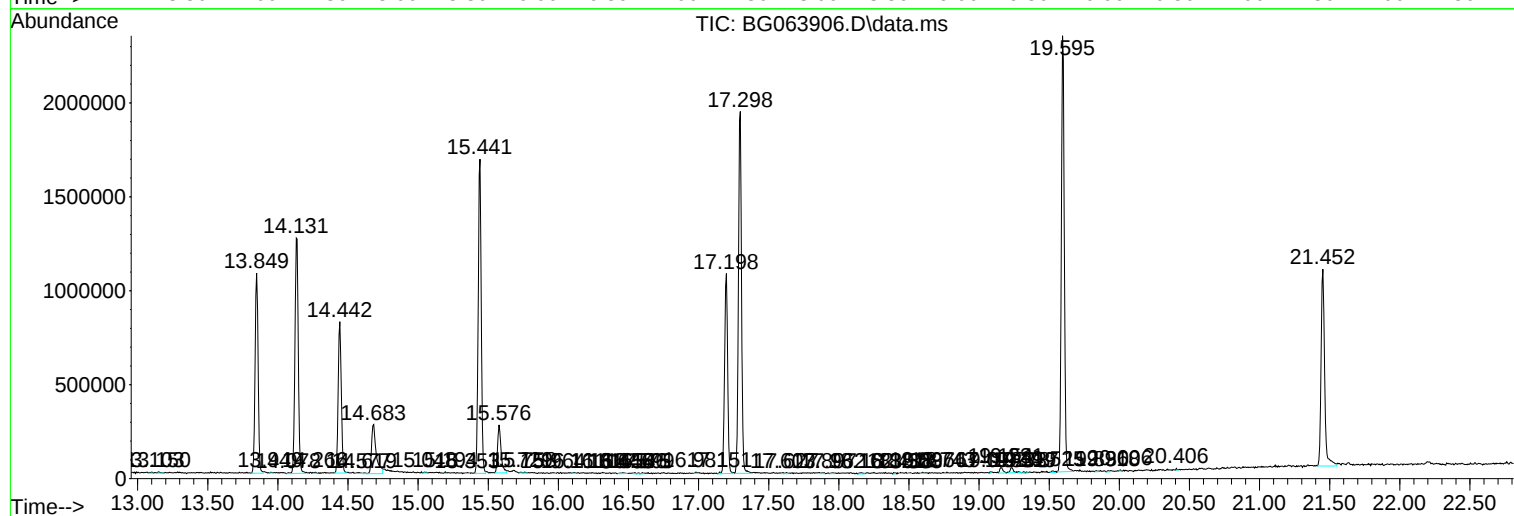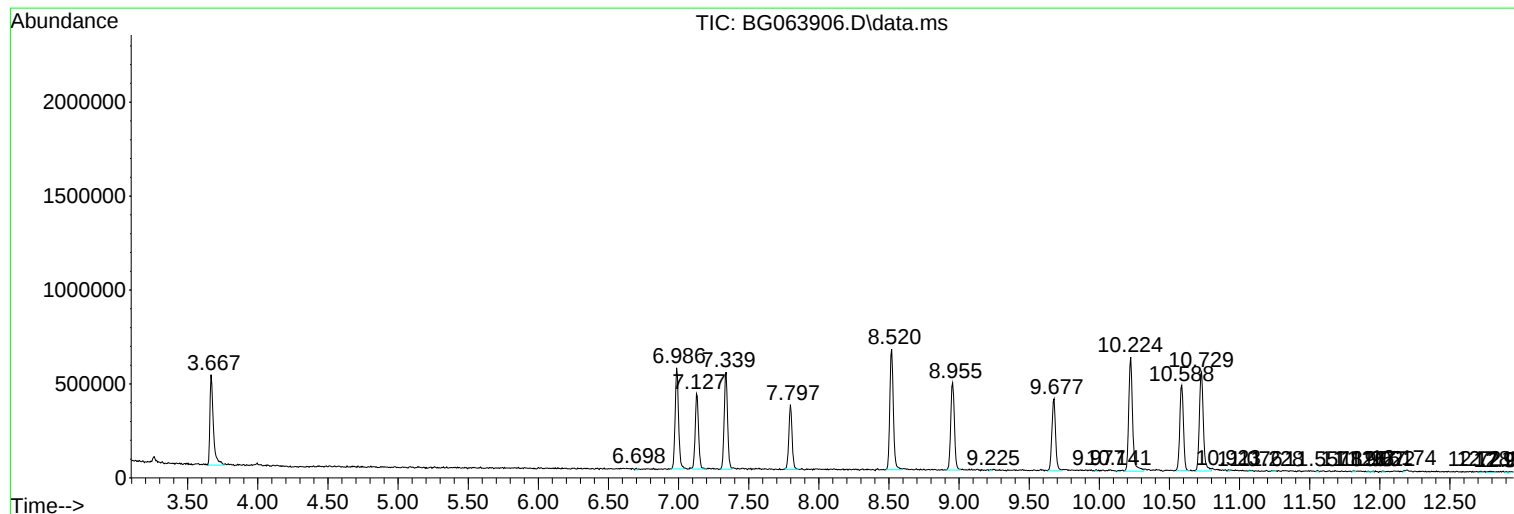

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063906.D
Acq On : 28 Dec 2024 16:37
Operator : RC/JU
Sample : PB165893BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122624\
Data File : BG063906.D
Acq On : 28 Dec 2024 16:37
Operator : RC/JU
Sample : PB165893BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc