
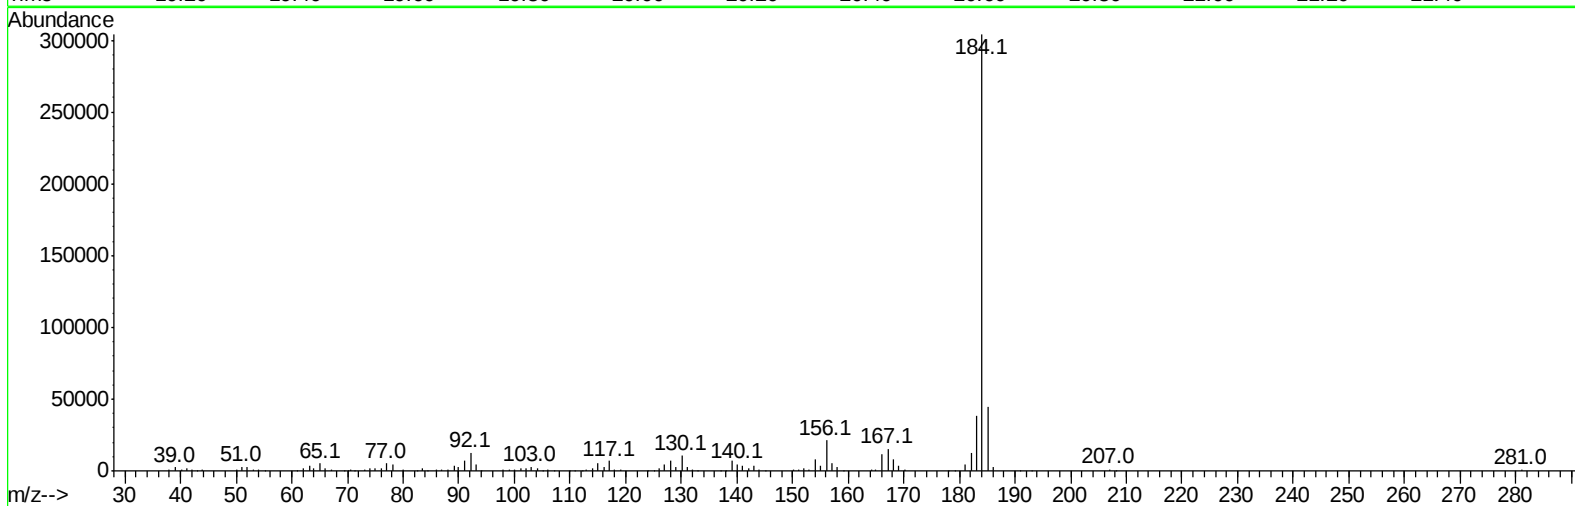


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
Data File : BG031793.D
Acq On : 27 Dec 2017 12:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 08:21:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

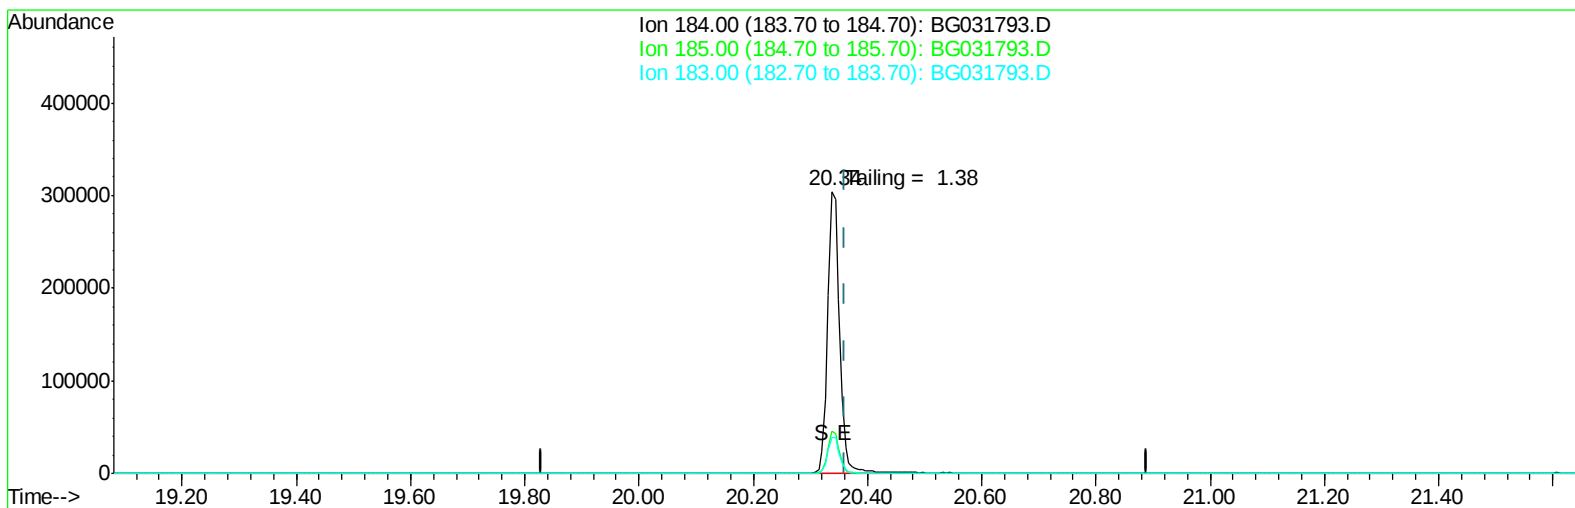

TIC: BG031793.D

(76) Benzidine



20.338min (-0.023) 0.00ng

response 437847

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.80
183.00	13.30	12.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
Data File : BG031793.D
Acq On : 27 Dec 2017 12:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 08:21:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

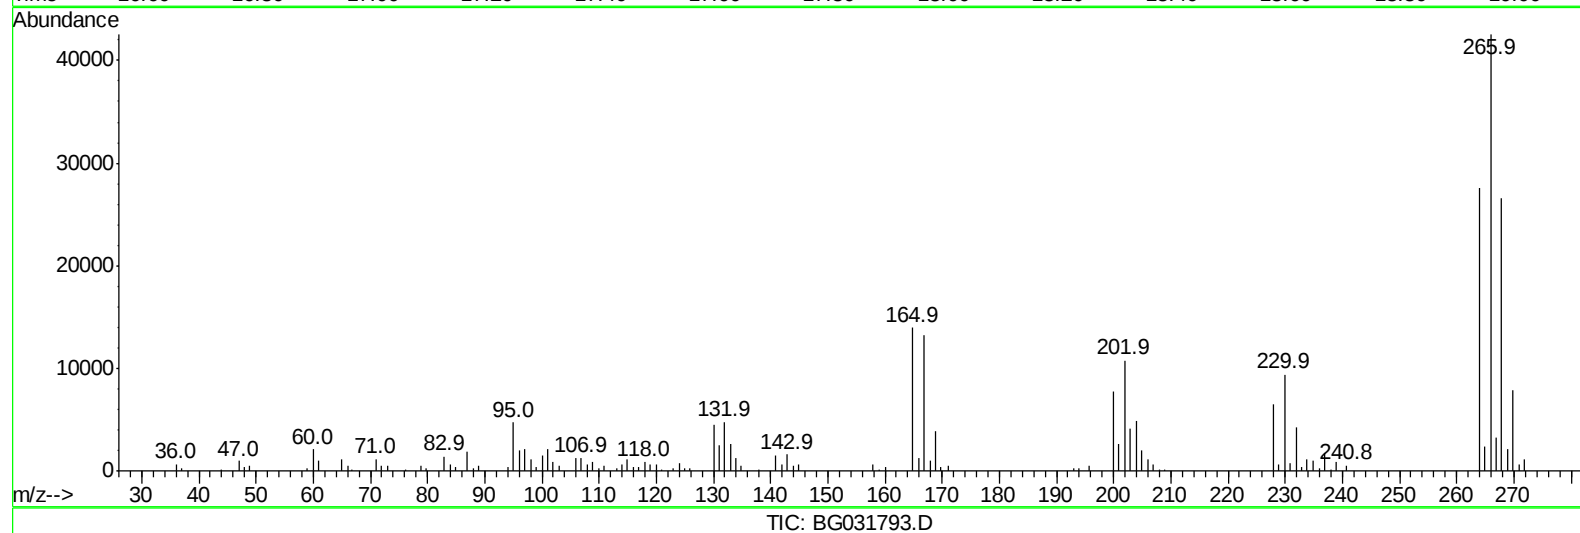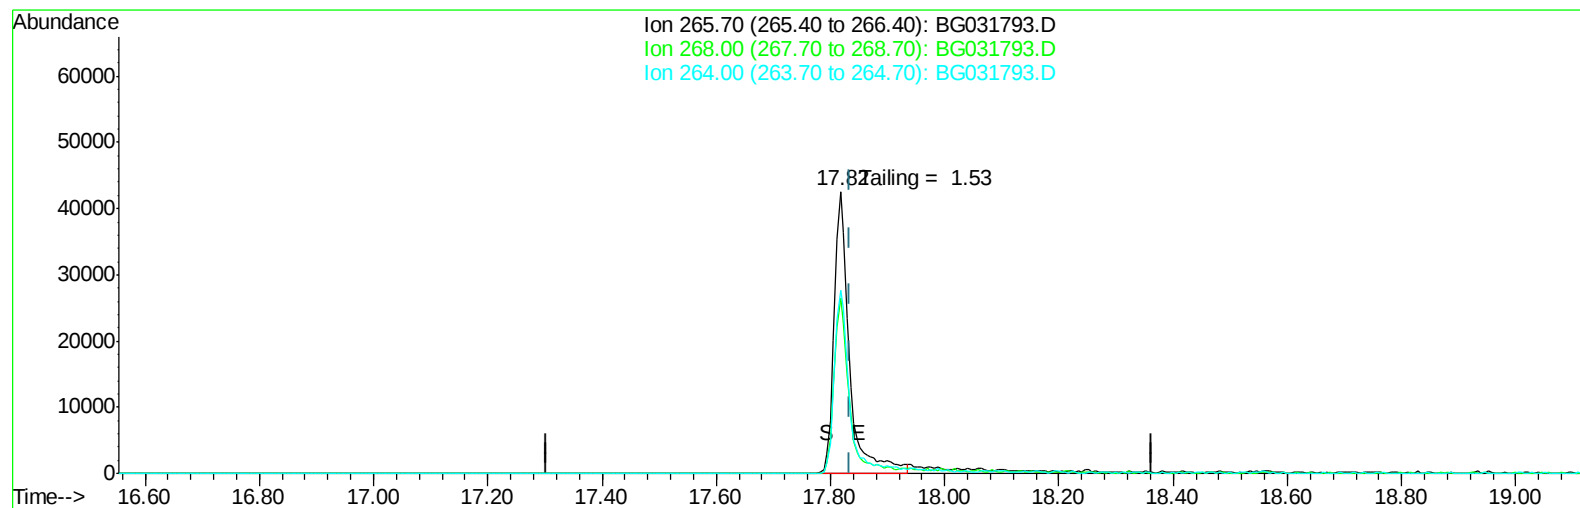

(69) Pentachlorophenol (C)

17.817min (-0.017) 19929.09ng

response 75785

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.35
264.00	62.00	64.80
0.00	0.00	0.00