
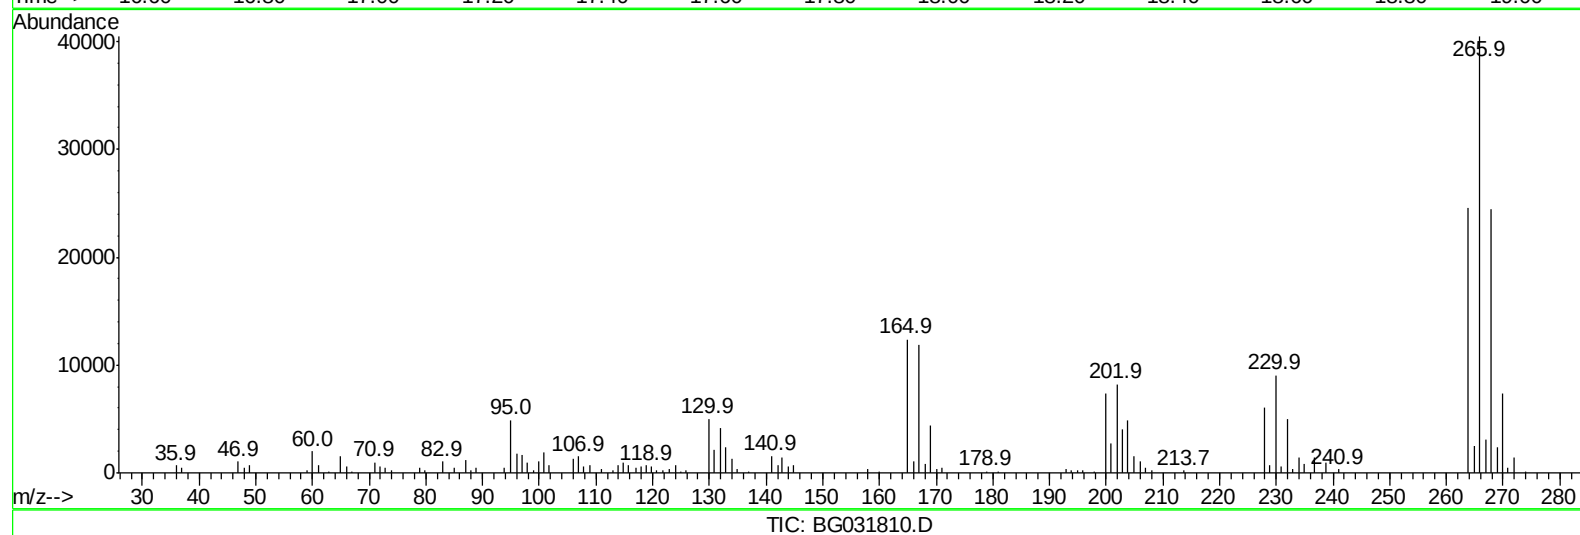


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\  
Data File : BG031810.D  
Acq On : 28 Dec 2017 00:14  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 08:22:43 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 11:08:55 2017  
Response via : Initial Calibration

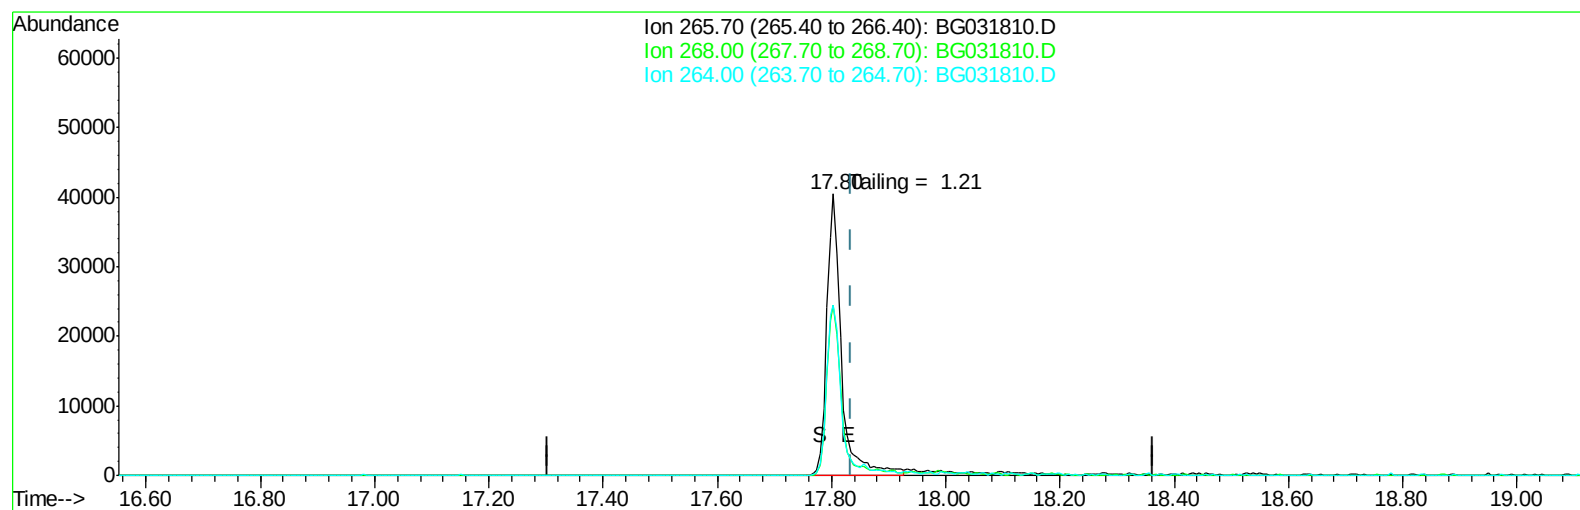

(69) Pentachlorophenol (C)



17.804min (-0.031) 22261.60ng

response 72432

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 60.51 |
| 264.00 | 62.00 | 60.69 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\  
Data File : BG031810.D  
Acq On : 28 Dec 2017 00:14  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 08:22:43 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 11:08:55 2017  
Response via : Initial Calibration

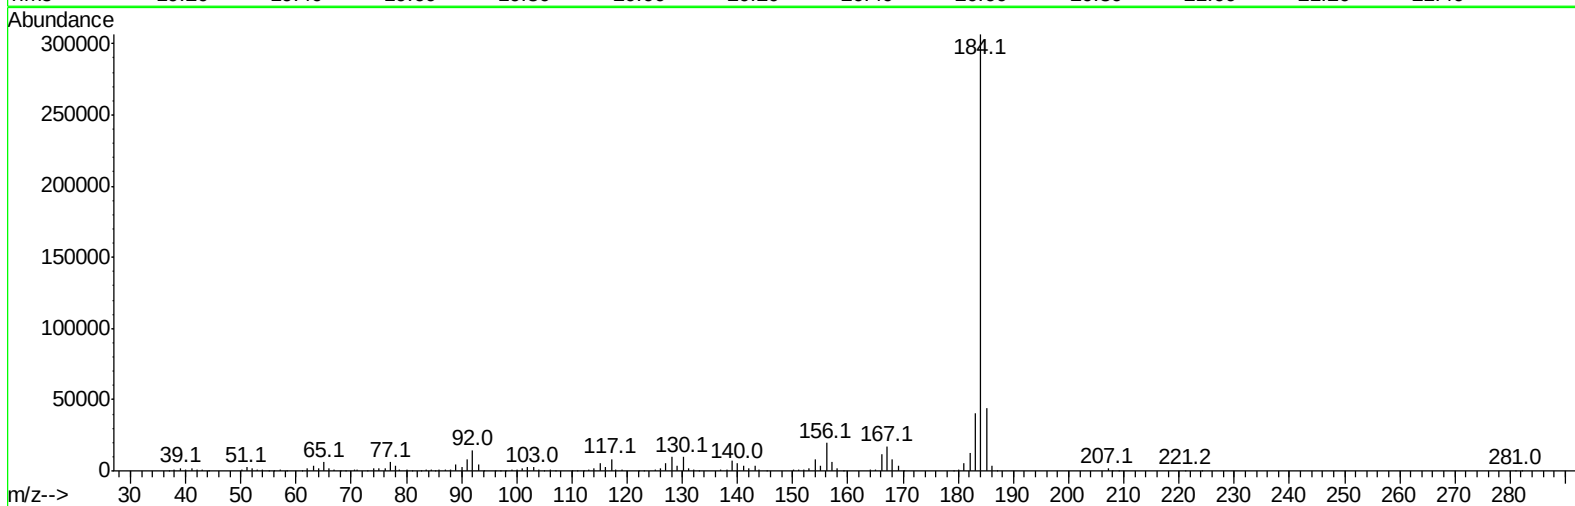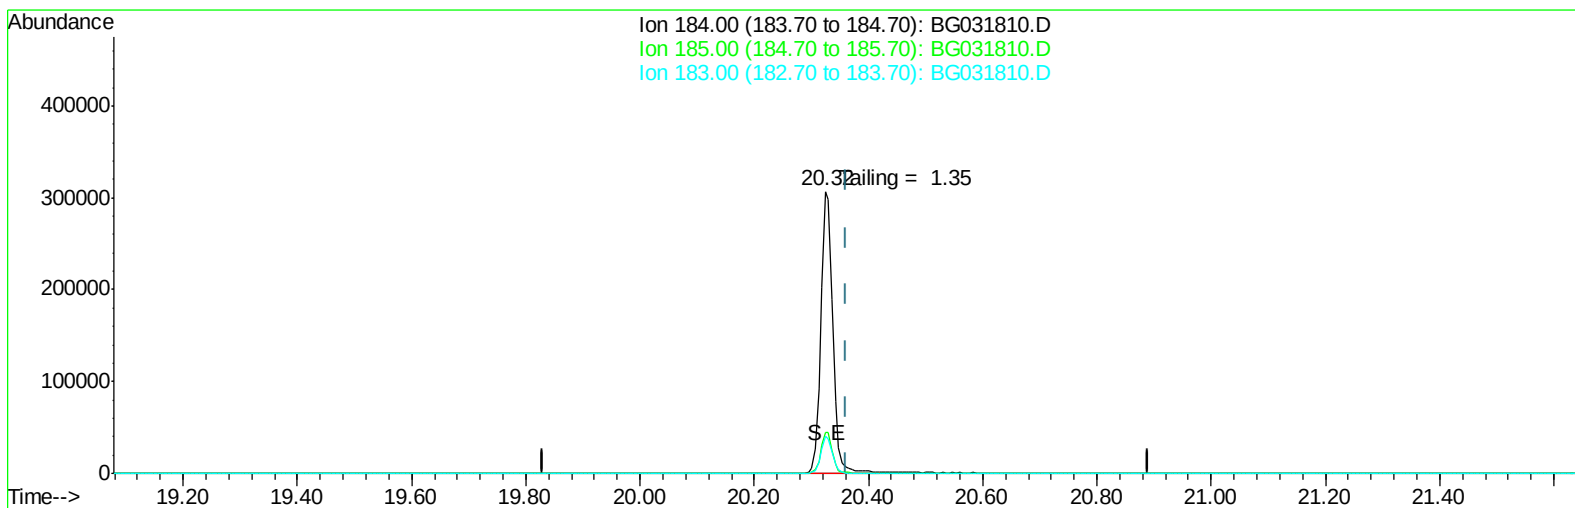

TIC: BG031810.D

(76) Benzidine

20.324min (-0.037) 0.00ng m

response 452766

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.51 |
| 183.00 | 13.30 | 13.34 |
| 0.00   | 0.00  | 0.00  |