

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
 Data File : BG031817.D
 Acq On : 28 Dec 2017 4:41
 Operator : SJ/JU
 Sample : I7010-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 122017-JETT-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.435	17	25	35	rBV	80692	168368	3.71%	0.999%
2	6.220	492	499	511	rBV	172691	304834	6.72%	1.810%
3	7.900	778	785	794	rVB	118354	212755	4.69%	1.263%
4	8.311	848	855	865	rBV	382807	691831	15.25%	4.107%
5	8.805	932	939	950	rVB	136879	244910	5.40%	1.454%
6	9.140	988	996	1009	rVB	576385	1069887	23.58%	6.351%
7	10.003	1132	1143	1157	rBV	404778	766159	16.89%	4.548%
8	11.690	1422	1430	1443	rVB	200015	370475	8.16%	2.199%
9	14.063	1825	1834	1844	rBV	1698393	2698674	59.48%	16.020%
10	15.432	2060	2067	2077	rVB2	379461	624007	13.75%	3.704%
11	16.202	2187	2198	2206	rBV	103900	166856	3.68%	0.990%
12	16.907	2310	2318	2330	rBV	916434	1480421	32.63%	8.788%
13	17.077	2338	2347	2354	rBV3	32132	63286	1.39%	0.376%
14	18.164	2525	2532	2544	rVB2	574534	895726	19.74%	5.317%
15	20.221	2877	2882	2892	rBV3	25049	48578	1.07%	0.288%
16	20.362	2901	2906	2913	rVB	56834	72251	1.59%	0.429%
17	20.697	2957	2963	2972	rBV	3186322	4537451	100.00%	26.935%
18	21.425	3083	3087	3091	rVB2	38113	46876	1.03%	0.278%
19	22.060	3188	3195	3204	rBV8	23704	47124	1.04%	0.280%
20	22.512	3264	3272	3282	rBV2	616432	1147229	25.28%	6.810%
21	26.267	3897	3911	3925	rBV2	357721	1187993	26.18%	7.052%


Sum of corrected areas: 16845691

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
Data File : BG031817.D
Acq On : 28 Dec 2017 4:41
Operator : SJ/JU
Sample : I7010-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
122017-JETT-F-D-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

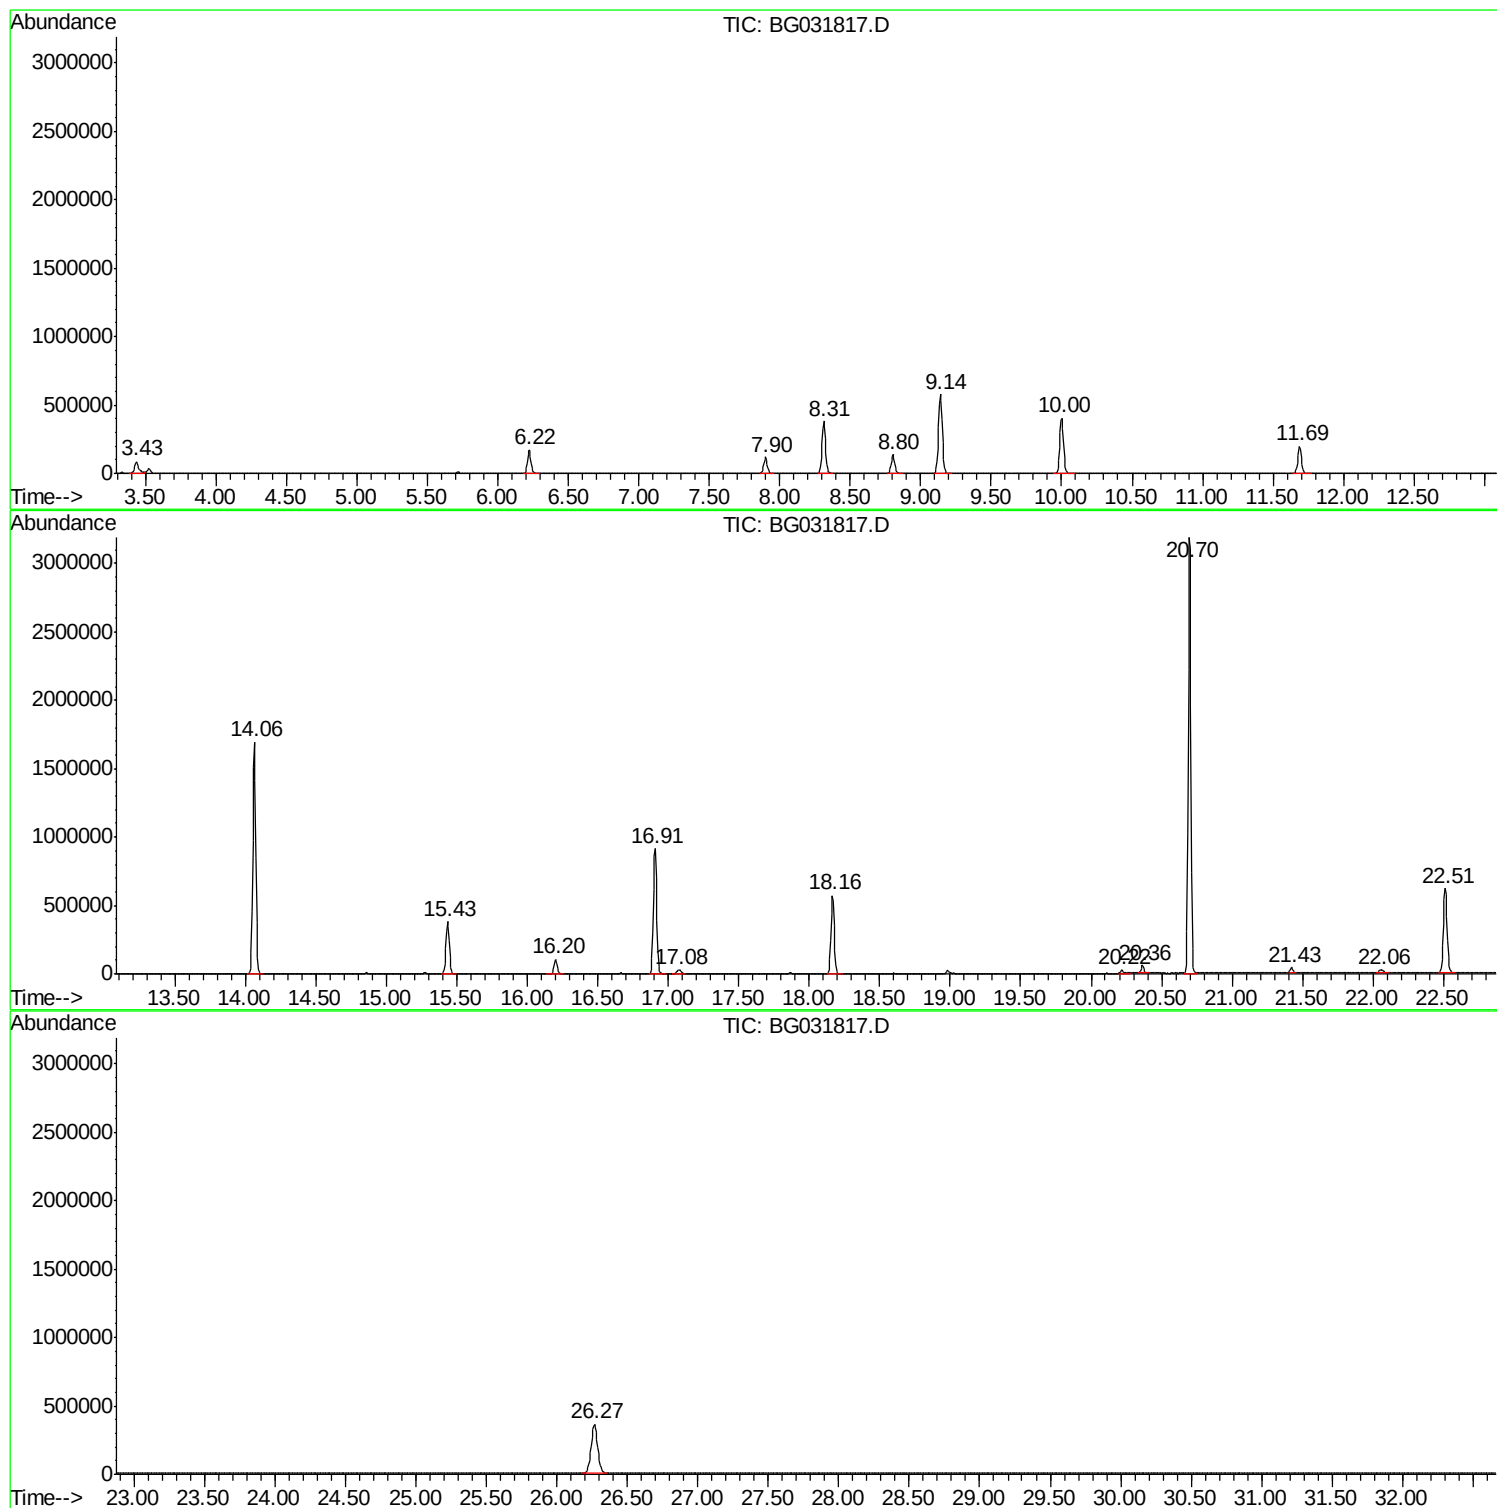

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG122717\
Data_File : BG031817.D
Acq_On : 28-Dec-2017 4:411
Operator : SJ/JUU
Sample : I7010-088
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
122017-JETT-F-D-M

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
