

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\  
 Data File : BG031818.D  
 Acq On : 28 Dec 2017 5:18  
 Operator : SJ/JU  
 Sample : I7010-09  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 122017-JETT-F-D-S

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG122117.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.434       | 19            | 25          | 37           | rBV2     | 91021          | 213243        | 4.81%           | 1.242%        |
| 2         | 3.528       | 37            | 41          | 49           | rVB2     | 28454          | 49186         | 1.11%           | 0.286%        |
| 3         | 6.225       | 493           | 500         | 513          | rBV      | 192880         | 330378        | 7.46%           | 1.923%        |
| 4         | 7.899       | 774           | 785         | 797          | rBV      | 117462         | 220188        | 4.97%           | 1.282%        |
| 5         | 8.317       | 846           | 856         | 866          | rBV      | 404373         | 748767        | 16.90%          | 4.359%        |
| 6         | 8.804       | 932           | 939         | 948          | rVB      | 162507         | 288285        | 6.51%           | 1.678%        |
| 7         | 9.139       | 986           | 996         | 1007         | rBV      | 608520         | 1159018       | 26.16%          | 6.748%        |
| 8         | 10.003      | 1134          | 1143        | 1155         | rBV      | 441540         | 825133        | 18.62%          | 4.804%        |
| 9         | 11.689      | 1420          | 1430        | 1440         | rBV      | 226801         | 423597        | 9.56%           | 2.466%        |
| 10        | 14.063      | 1826          | 1834        | 1845         | rVB      | 1780943        | 2833787       | 63.96%          | 16.498%       |
| 11        | 15.432      | 2061          | 2067        | 2075         | rVB2     | 408690         | 684108        | 15.44%          | 3.983%        |
| 12        | 16.906      | 2311          | 2318        | 2330         | rBV      | 996729         | 1571905       | 35.48%          | 9.152%        |
| 13        | 17.077      | 2342          | 2347        | 2357         | rVB3     | 29172          | 45871         | 1.04%           | 0.267%        |
| 14        | 18.164      | 2525          | 2532        | 2542         | rBV      | 590714         | 932298        | 21.04%          | 5.428%        |
| 15        | 20.361      | 2902          | 2906        | 2912         | rVB      | 46685          | 55806         | 1.26%           | 0.325%        |
| 16        | 20.696      | 2957          | 2963        | 2974         | rBV      | 3144471        | 4430650       | 100.00%         | 25.795%       |
| 17        | 22.512      | 3265          | 3272        | 3282         | rVB2     | 628537         | 1173543       | 26.49%          | 6.832%        |
| 18        | 26.260      | 3896          | 3910        | 3923         | rBV3     | 359683         | 1190395       | 26.87%          | 6.931%        |


Sum of corrected areas: 17176158

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\  
Data File : BG031818.D  
Acq On : 28 Dec 2017 5:18  
Operator : SJ/JU  
Sample : I7010-09  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
122017-JETT-F-D-S

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

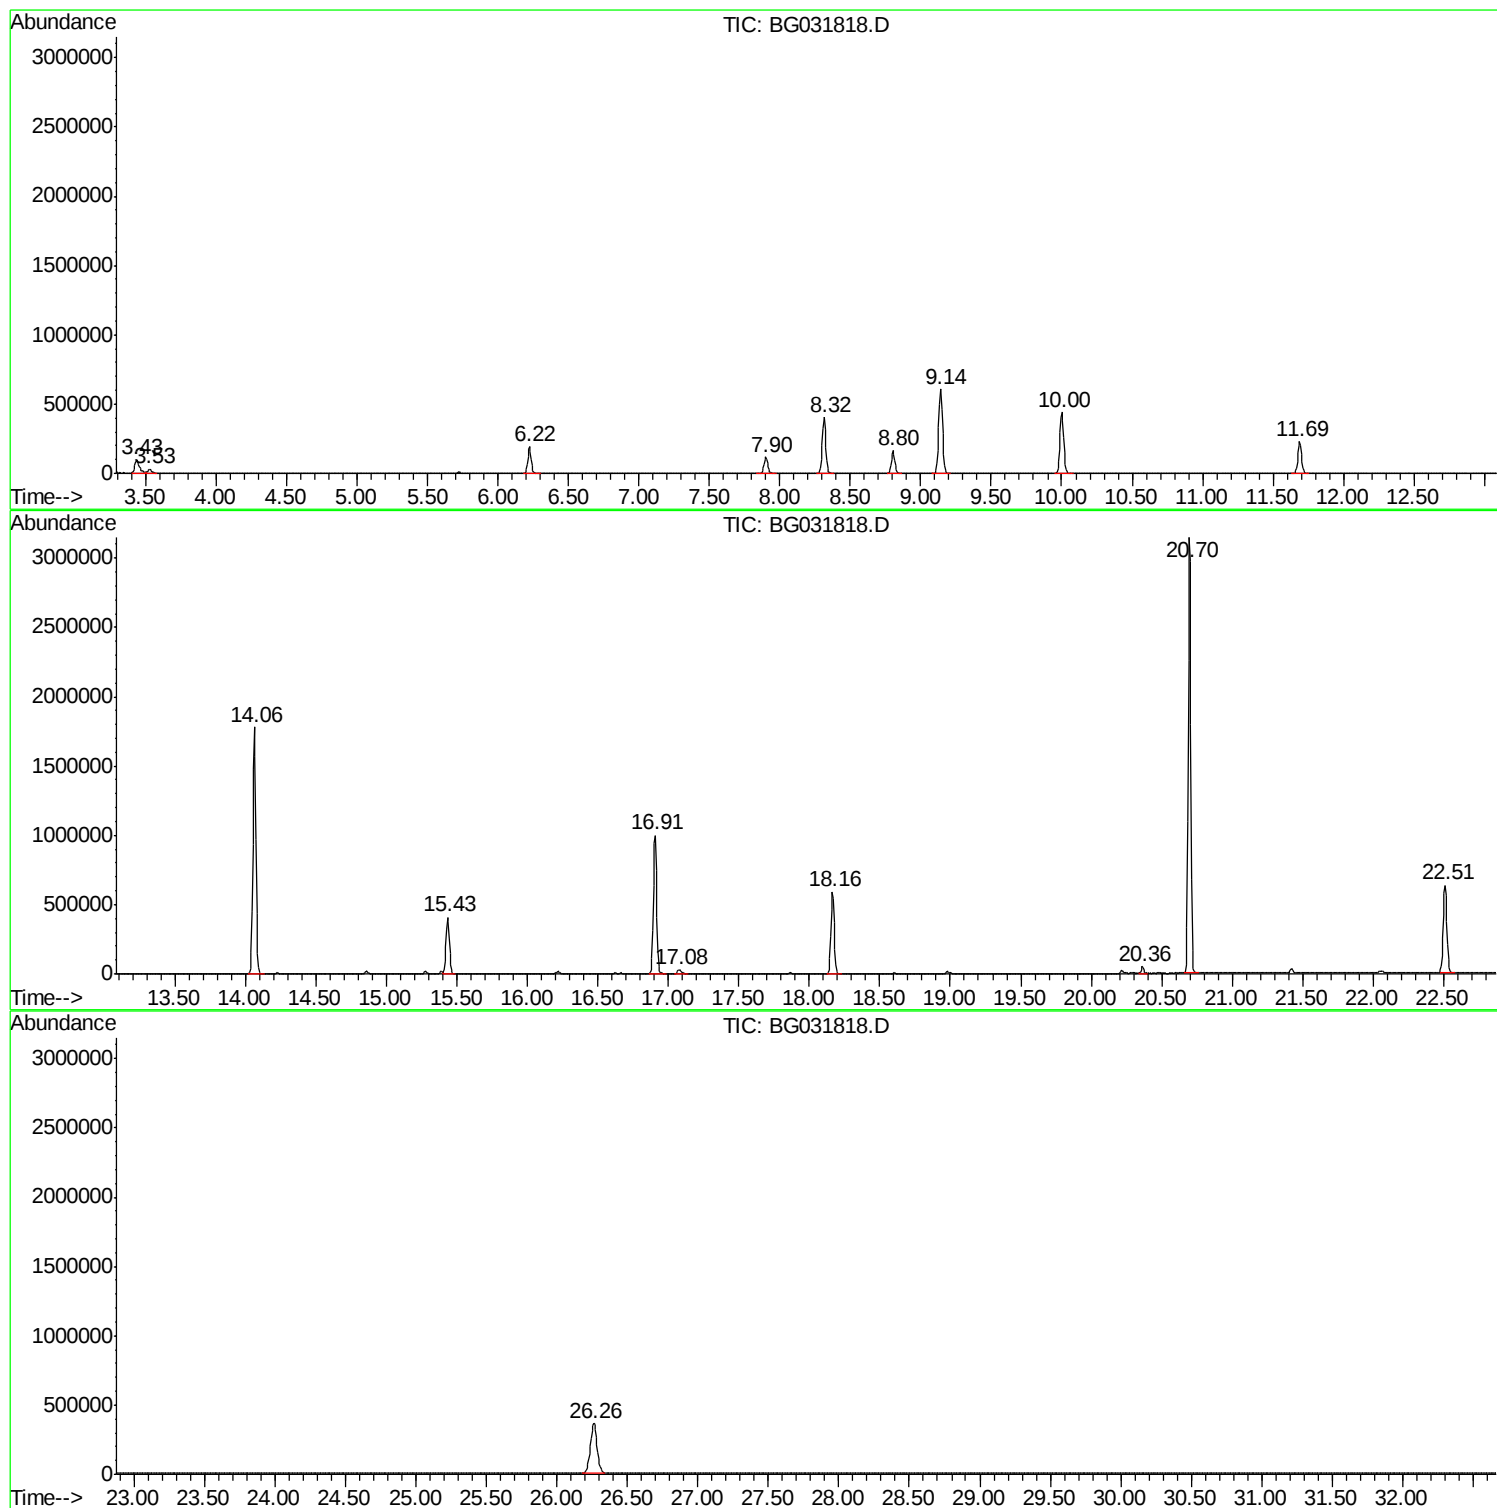

Data\_Path : Z:\HPCHEM1\BNA\_G\DATA\BG122717\  
Data\_File : BG031818.D  
Acq\_On : 28-Dec-2017 5:188  
Operator : SJ/JUU  
Sample : I7010-099  
Misc :  
ALS\_Vial : 24 Sample\_Multiplier: 11

Instrument :  
BNA\_G  
ClientSampleId :  
122017-JETT-F-D-S

Quant\_Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG122117.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC\_Library : C:\Database\NIST11.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|

No Library Search Compounds Detected

\*\*\*\*\*