

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
 Data File : BG031819.D
 Acq On : 28 Dec 2017 5:56
 Operator : SJ/JU
 Sample : I7010-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 122017-JETT-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	16	25	35	rBV2	90168	210569	4.91%	1.244%
2	3.528	36	41	49	rVB	30720	51517	1.20%	0.304%
3	6.225	491	500	510	rBV	186530	321949	7.50%	1.902%
4	7.899	778	785	796	rBV	115699	223378	5.20%	1.320%
5	8.311	848	855	868	rBV	389248	724254	16.87%	4.278%
6	8.804	931	939	948	rBV2	154118	281457	6.56%	1.663%
7	9.139	987	996	1009	rVB	612682	1136441	26.48%	6.713%
8	10.003	1134	1143	1153	rBV	435532	813523	18.95%	4.806%
9	11.689	1420	1430	1441	rBV	217672	406988	9.48%	2.404%
10	14.063	1826	1834	1844	rBV	1703756	2732150	63.66%	16.140%
11	15.432	2058	2067	2077	rVB2	377698	646541	15.06%	3.819%
12	16.201	2189	2198	2205	rBV	122742	203717	4.75%	1.203%
13	16.906	2310	2318	2331	rBV	890669	1457854	33.97%	8.612%
14	17.077	2339	2347	2358	rVB4	29883	64097	1.49%	0.379%
15	18.164	2525	2532	2541	rBV2	577242	902241	21.02%	5.330%
16	18.980	2667	2671	2679	rBV2	32590	50804	1.18%	0.300%
17	20.214	2877	2881	2890	rBV3	32982	57545	1.34%	0.340%
18	20.696	2957	2963	2971	rBV	3121560	4291993	100.00%	25.355%
19	22.053	3187	3194	3199	rBV5	27091	46362	1.08%	0.274%
20	22.512	3264	3272	3283	rBV2	604926	1149418	26.78%	6.790%
21	26.260	3897	3910	3927	rVB2	345594	1154977	26.91%	6.823%


Sum of corrected areas: 16927775

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
Data File : BG031819.D
Acq On : 28 Dec 2017 5:56
Operator : SJ/JU
Sample : I7010-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
122017-JETT-F-U-B

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

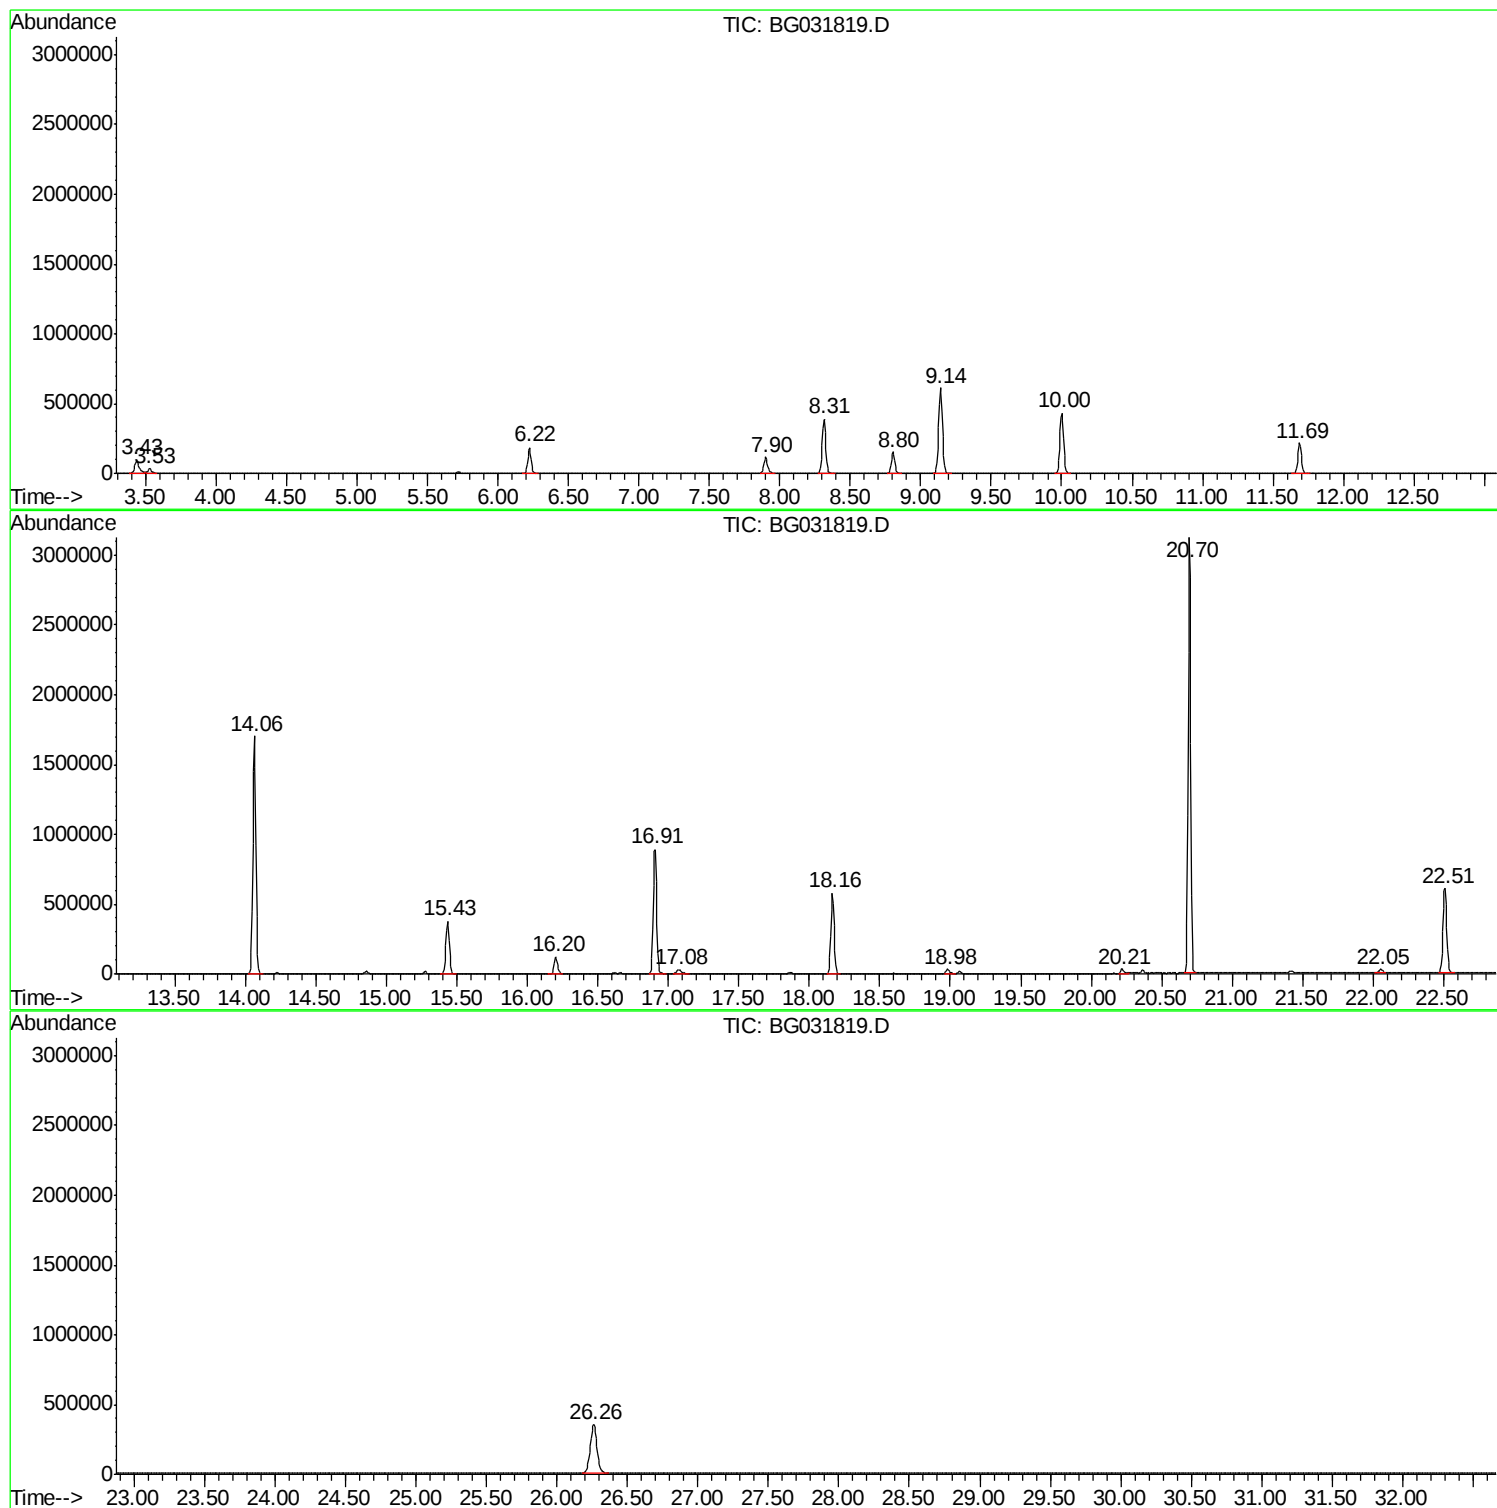

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG122717\
Data_File : BG031819.D
Acq_On : 28-Dec-2017 5:566
Operator : SJ/JUU
Sample : I7010-100
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
122017-JETT-F-U-B

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
