


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
 Data File : BG031793.D
 Acq On : 27 Dec 2017 12:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

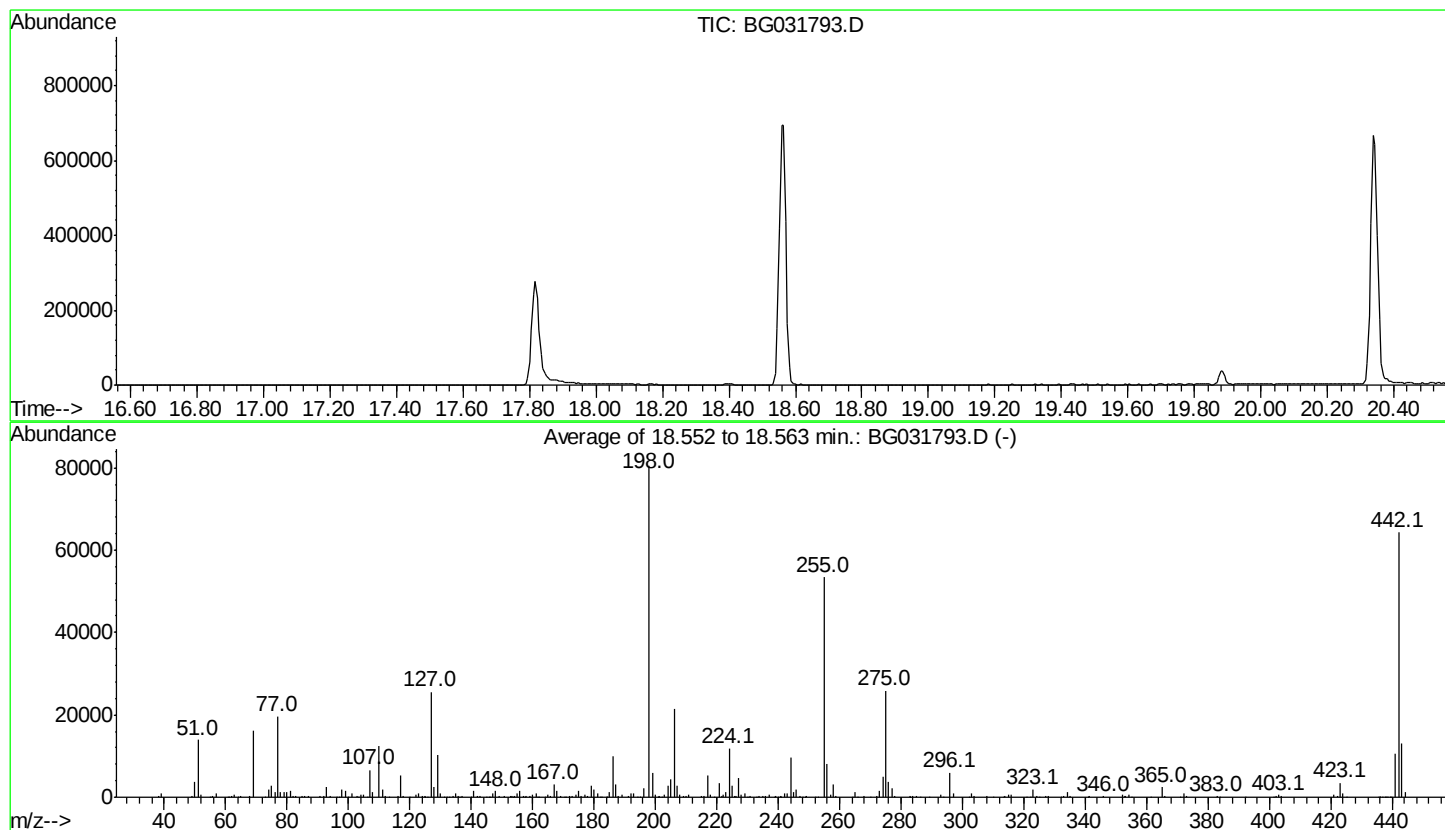

AutoFind: Scans 2598, 2599, 2600; Background Corrected with Scan 2592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.3	13891	PASS
68	69	0.00	2	1.6	264	PASS
69	198	0.00	100	20.2	16262	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.8	25602	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80525	PASS
199	198	5	9	7.3	5877	PASS
275	198	10	60	32.2	25933	PASS
365	198	1	100	3.0	2413	PASS
441	442	0.01	24	16.4	10529	PASS
442	198	50	100	79.9	64317	PASS
443	442	15	24	20.2	13024	PASS