


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122717\
 Data File : BG031810.D
 Acq On : 28 Dec 2017 00:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

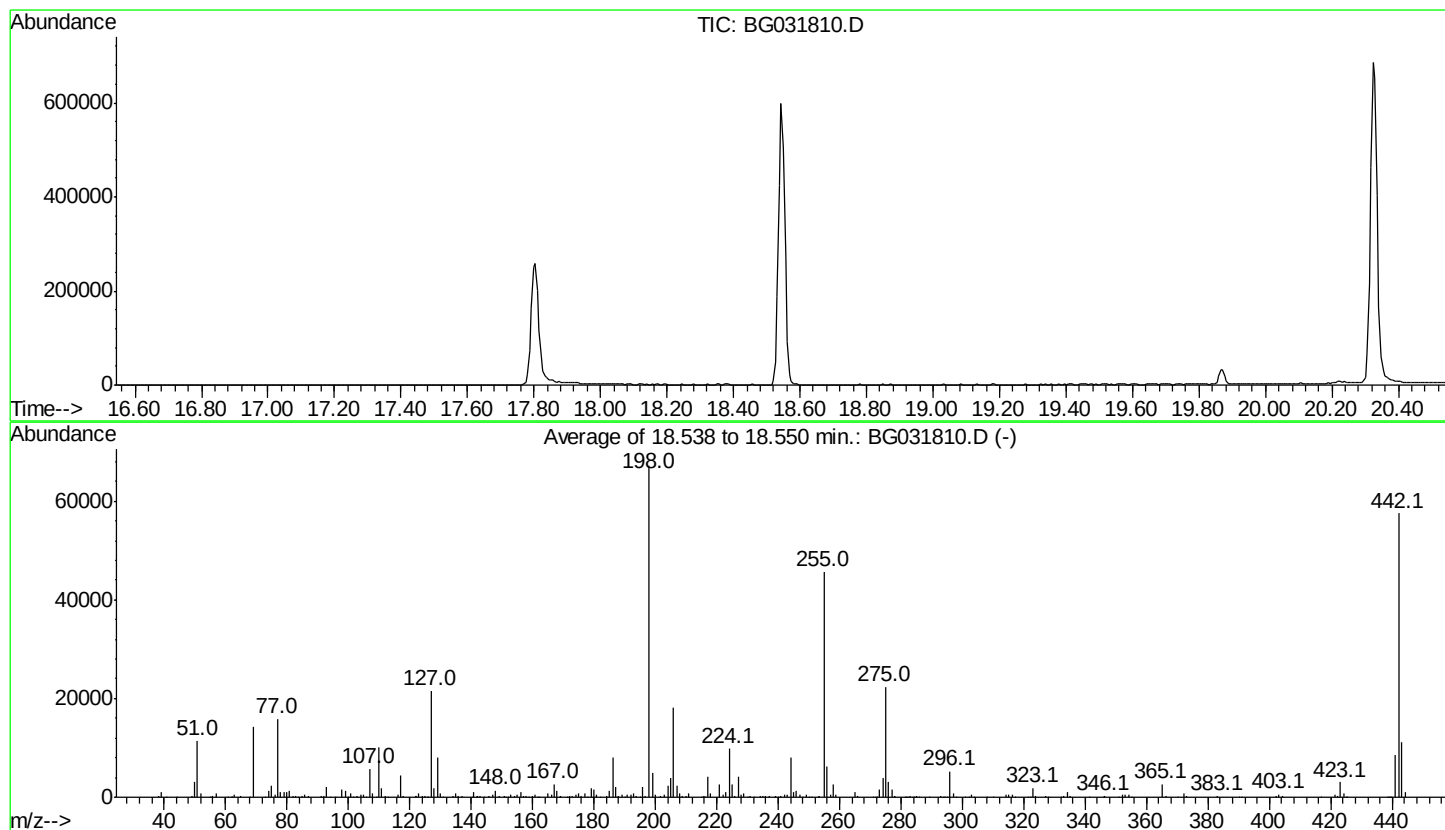

AutoFind: Scans 2595, 2596, 2597; Background Corrected with Scan 2589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.2	11543	PASS
68	69	0.00	2	0.6	85	PASS
69	198	0.00	100	21.3	14300	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.2	21634	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67181	PASS
199	198	5	9	7.3	4890	PASS
275	198	10	60	33.4	22416	PASS
365	198	1	100	4.0	2715	PASS
441	442	0.01	24	15.0	8590	PASS
442	198	50	100	85.5	57453	PASS
443	442	15	24	19.2	11050	PASS