
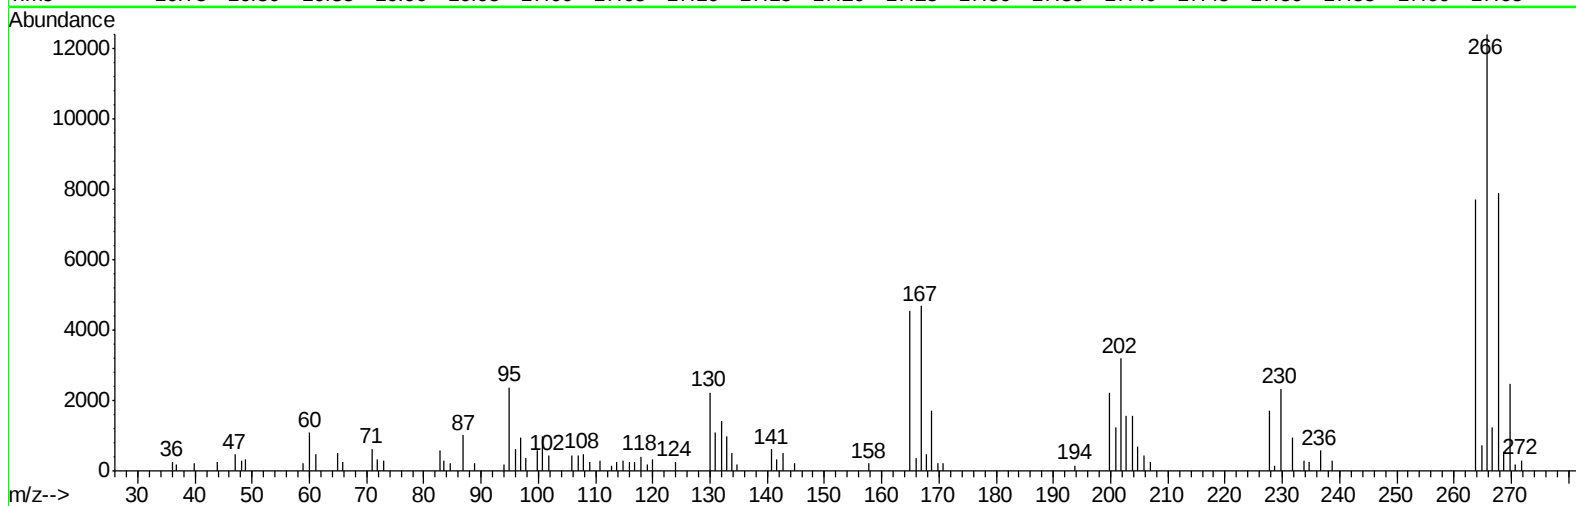


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122718\
Data File : BG038859.D
Acq On : 28 Dec 2018 1:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:53:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

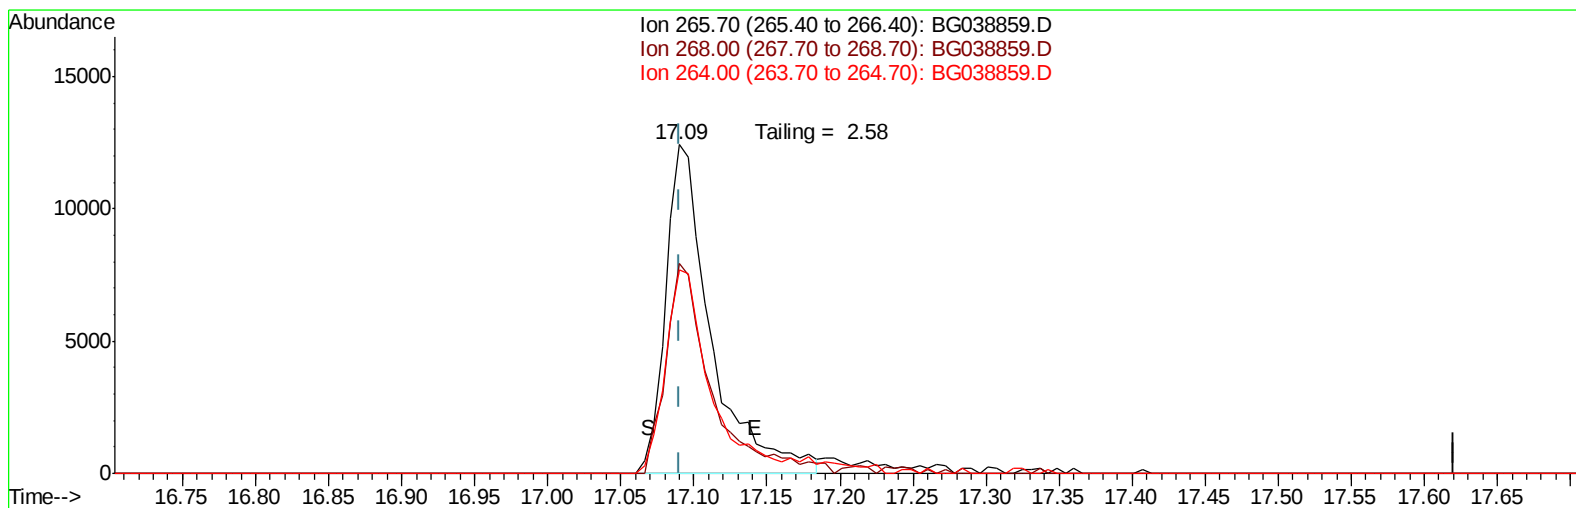

TIC: BG038859.D

(70) Pentachlorophenol (C)



17.090min (-0.000) 0.00ng

response 27616

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.26
264.00	70.90	62.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122718\
Data File : BG038859.D
Acq On : 28 Dec 2018 1:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:53:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

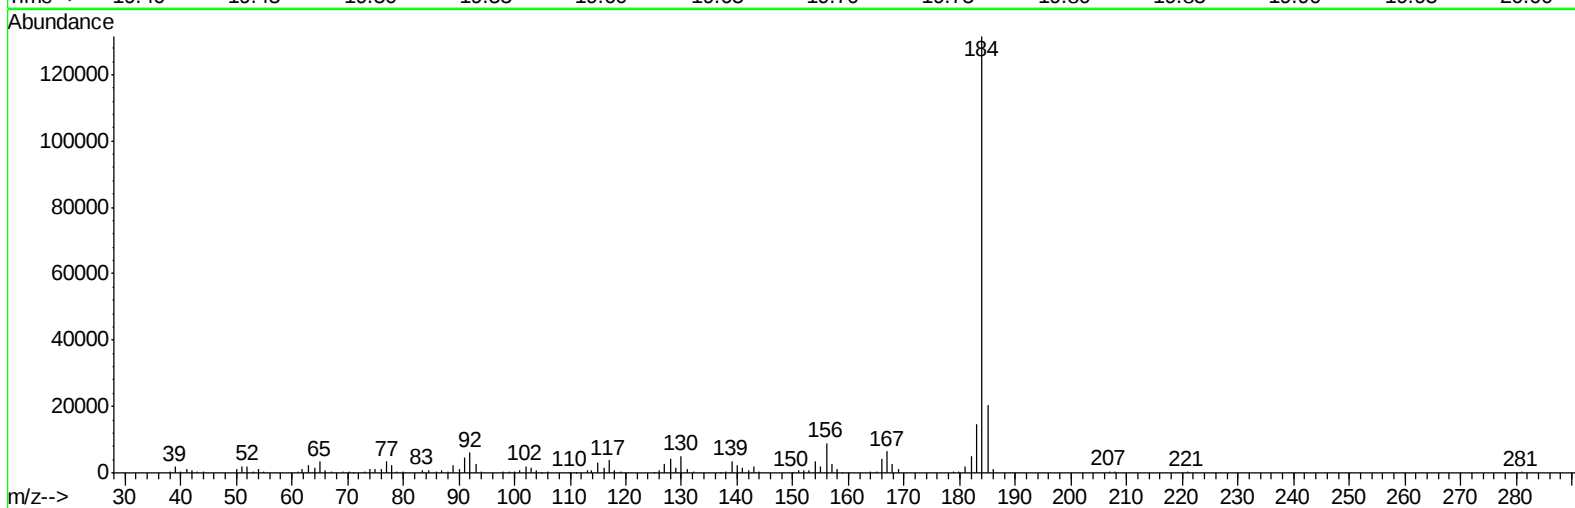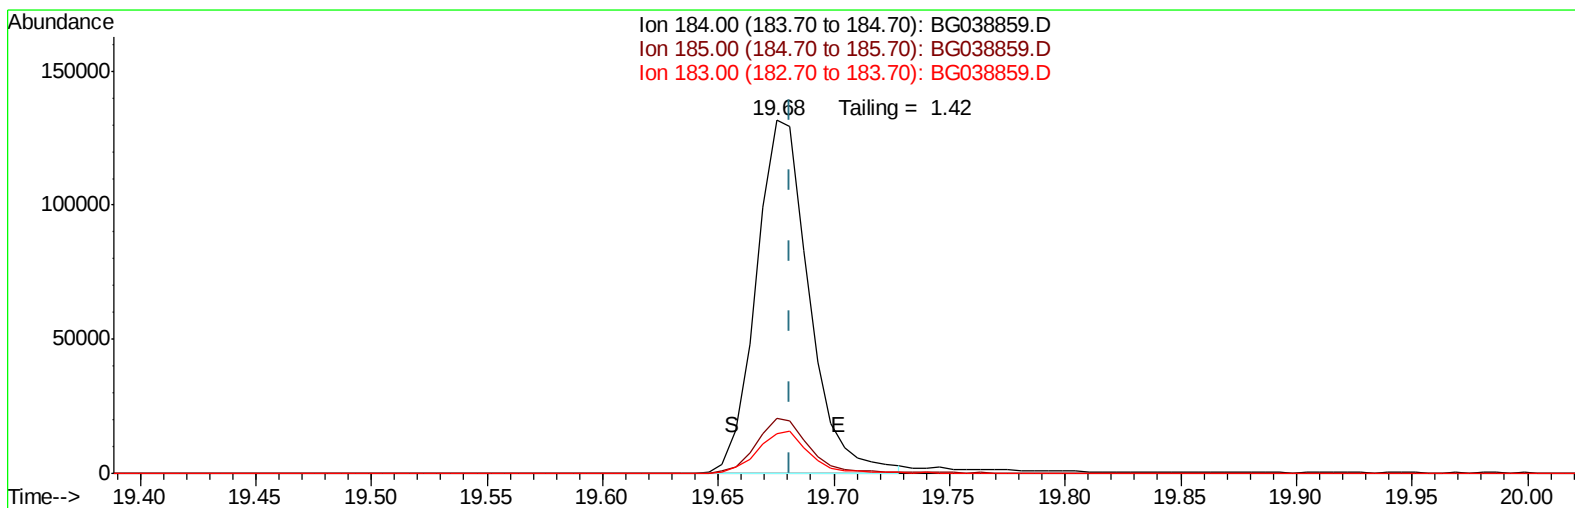

TIC: BG038859.D

(77) Benzidine

19.675min (-0.006) 0.00ng

response 217805

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.63
183.00	12.00	11.30
0.00	0.00	0.00