


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122718\
 Data File : BG038839.D
 Acq On : 27 Dec 2018 9:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

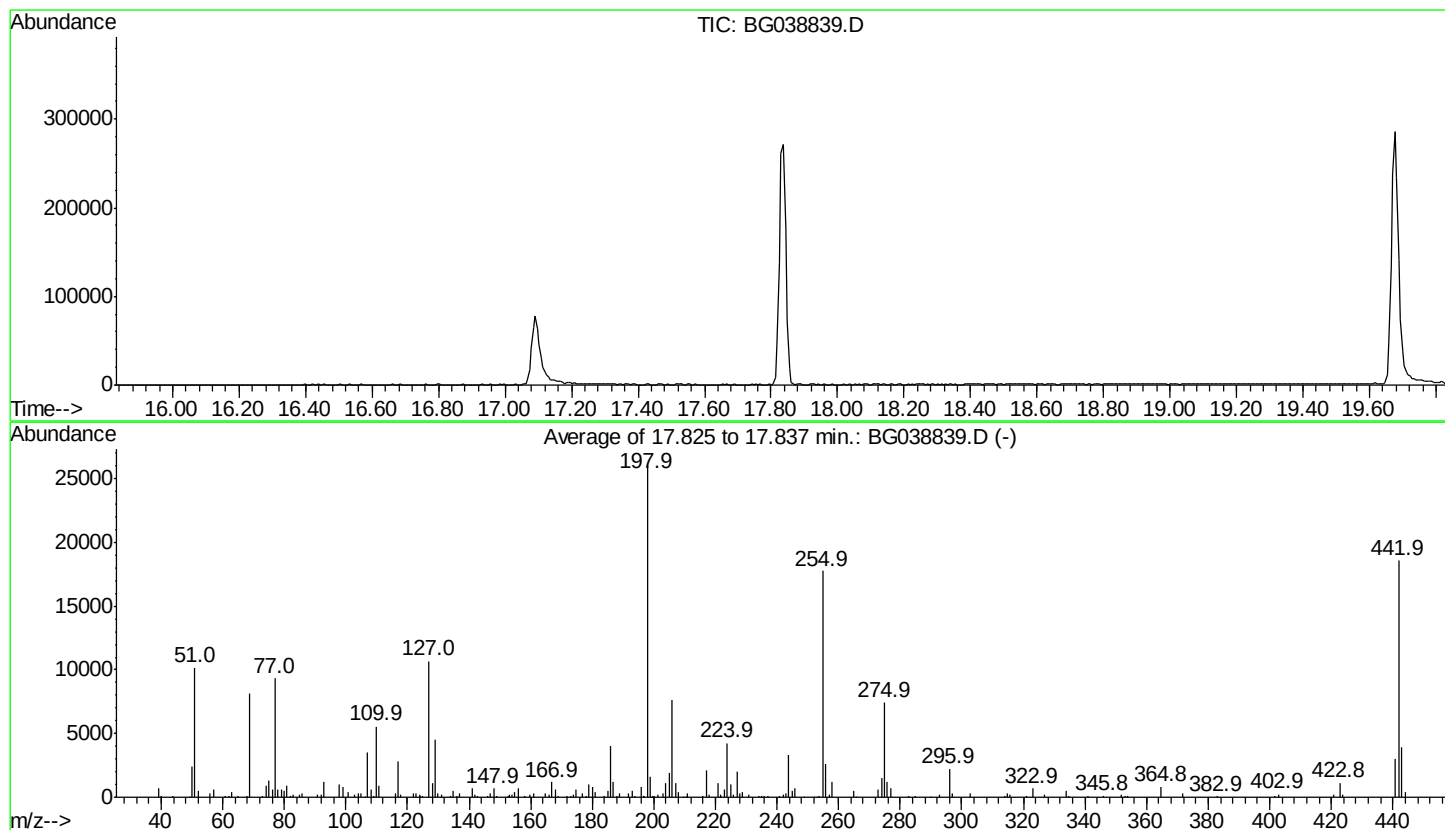

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	10191	PASS
68	69	0.00	2	1.0	78	PASS
69	198	0.00	100	31.3	8133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	10683	PASS
197	198	0.00	2	0.4	112	PASS
198	198	100	100	100.0	26016	PASS
199	198	5	9	6.2	1611	PASS
275	198	10	60	28.5	7419	PASS
365	198	1	100	3.2	835	PASS
441	198	0.01	100	11.4	2967	PASS
442	198	50	100	71.4	18575	PASS
443	442	15	24	21.2	3938	PASS