


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122718\  
 Data File : BG038842.D  
 Acq On : 27 Dec 2018 13:28  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG121218.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Dec 12 15:26:27 2018

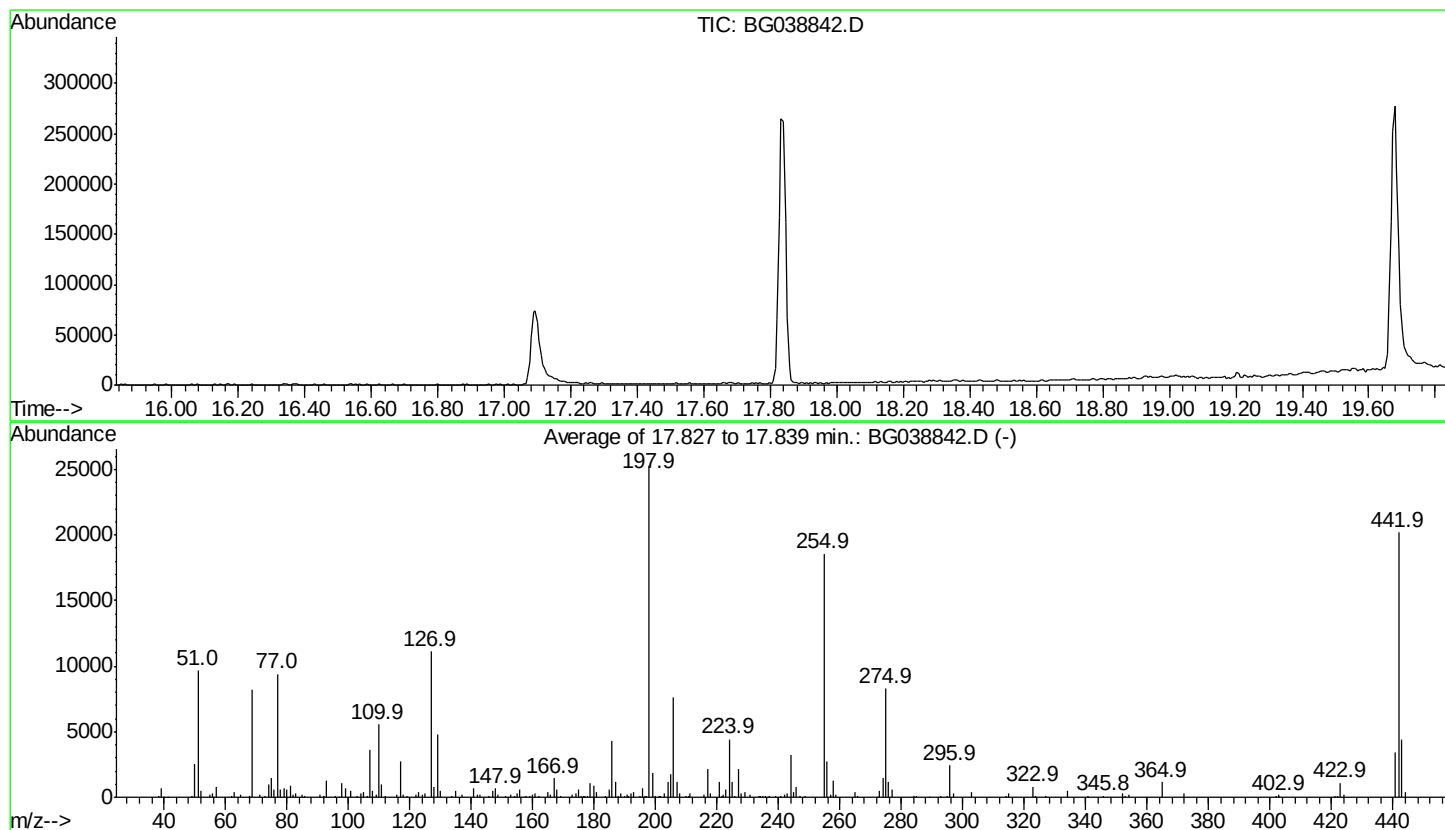

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 38.1      | 9638    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.2       | 102     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.4      | 8182    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 44.0      | 11108   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 122     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 25272   | PASS             |
| 199         | 198          | 5            | 9            | 7.3       | 1833    | PASS             |
| 275         | 198          | 10           | 60           | 32.7      | 8254    | PASS             |
| 365         | 198          | 1            | 100          | 4.5       | 1135    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.6      | 3431    | PASS             |
| 442         | 198          | 50           | 100          | 79.8      | 20158   | PASS             |
| 443         | 442          | 15           | 24           | 21.7      | 4380    | PASS             |