


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122718\
 Data File : BG038859.D
 Acq On : 28 Dec 2018 1:48
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

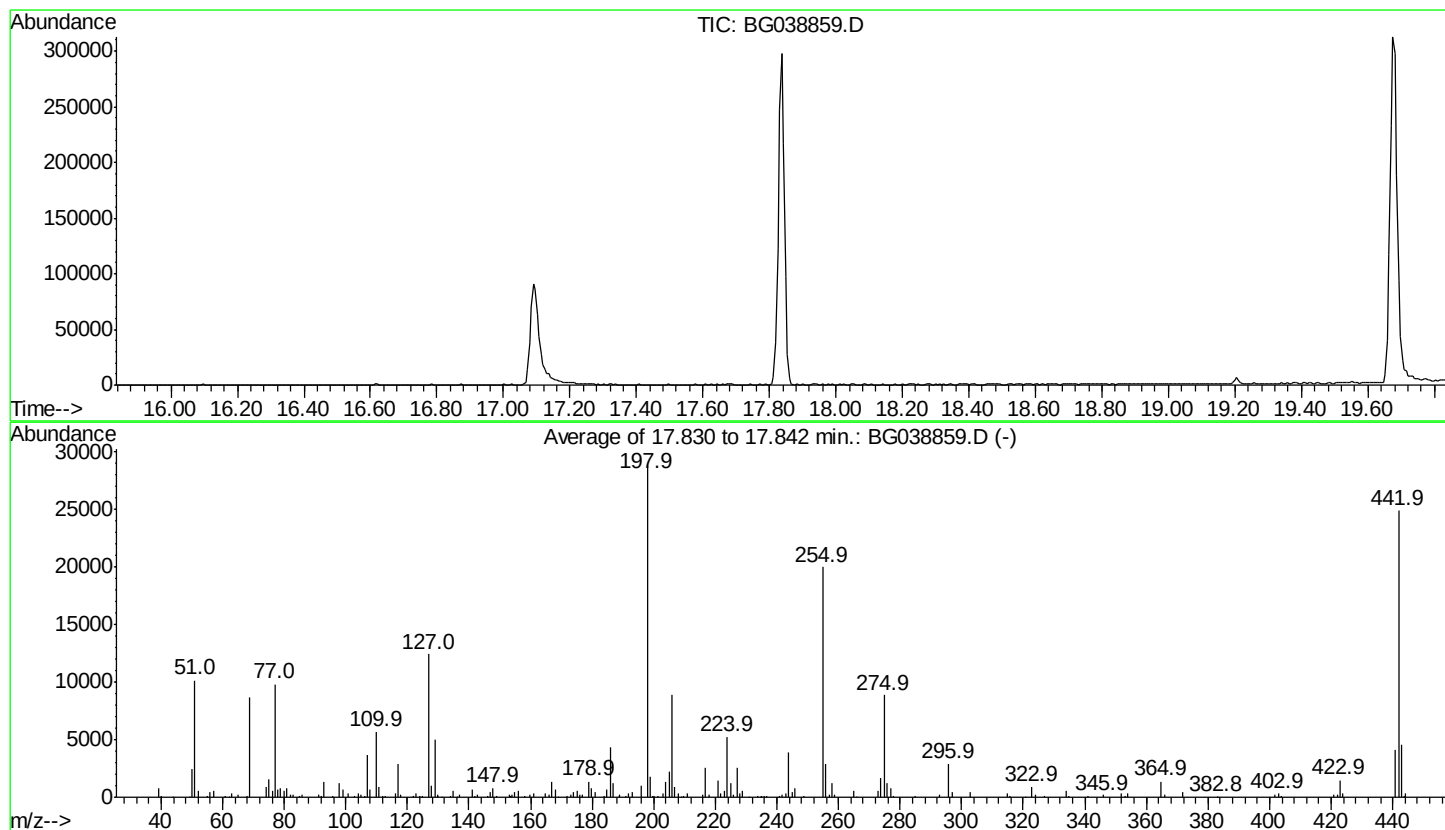

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	10108	PASS
68	69	0.00	2	1.8	156	PASS
69	198	0.00	100	30.2	8687	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	12425	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28768	PASS
199	198	5	9	6.1	1753	PASS
275	198	10	60	30.8	8870	PASS
365	198	1	100	4.7	1341	PASS
441	198	0.01	100	14.3	4124	PASS
442	198	50	100	86.3	24826	PASS
443	442	15	24	18.5	4589	PASS