
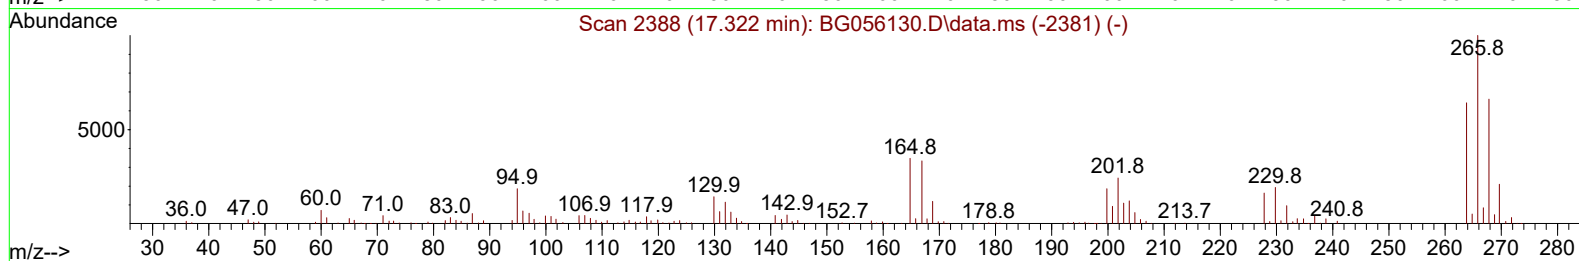
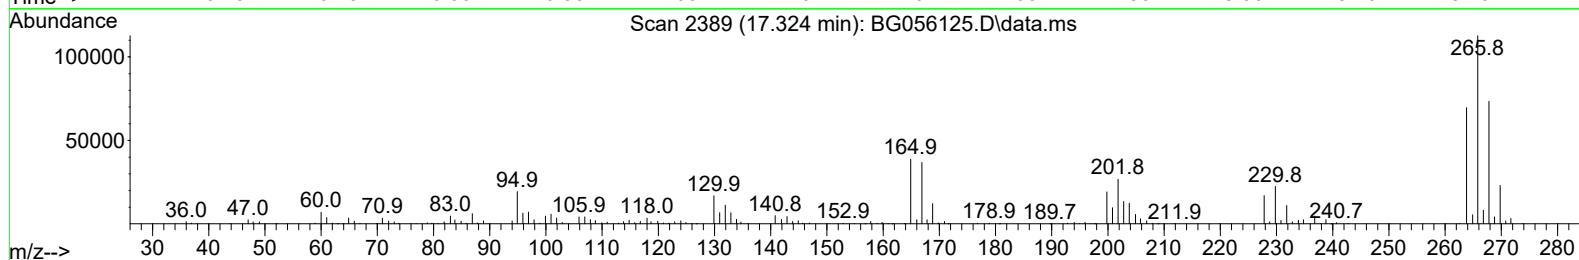


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122722\
Data File : BG056125.D
Acq On : 27 Dec 2022 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:08:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

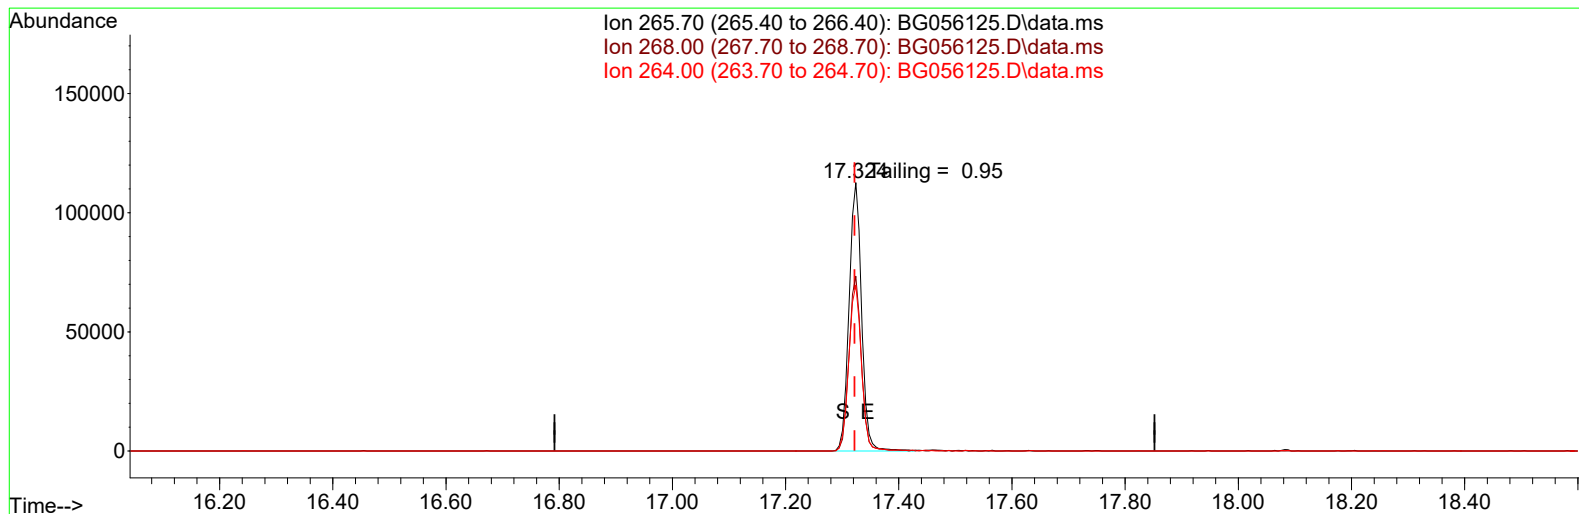

TIC: BG056125.D\data.ms

(70) Pentachlorophenol (C)




17.324min (+ 0.002) 311339.09 ng

response 173323

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.12
264.00	64.30	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122722\
Data File : BG056125.D
Acq On : 27 Dec 2022 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:08:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

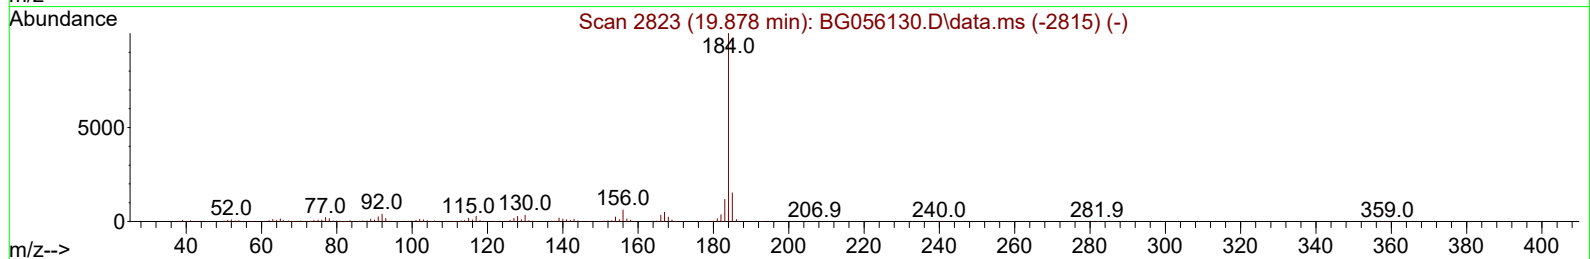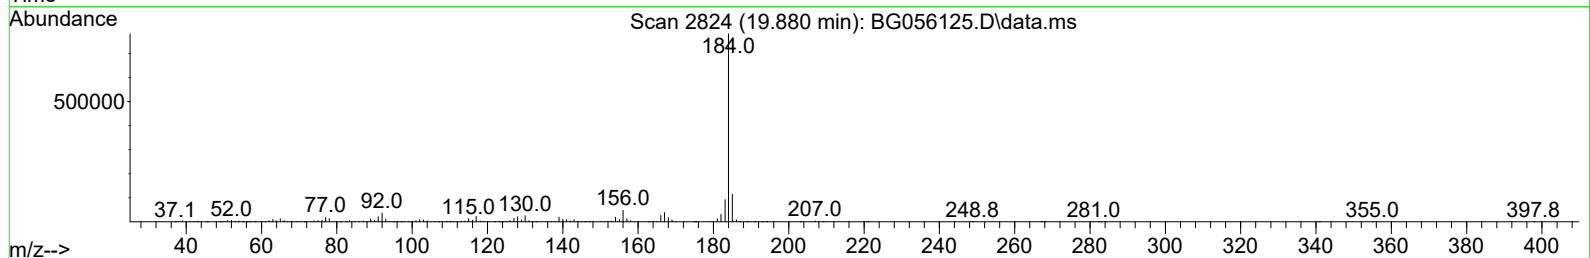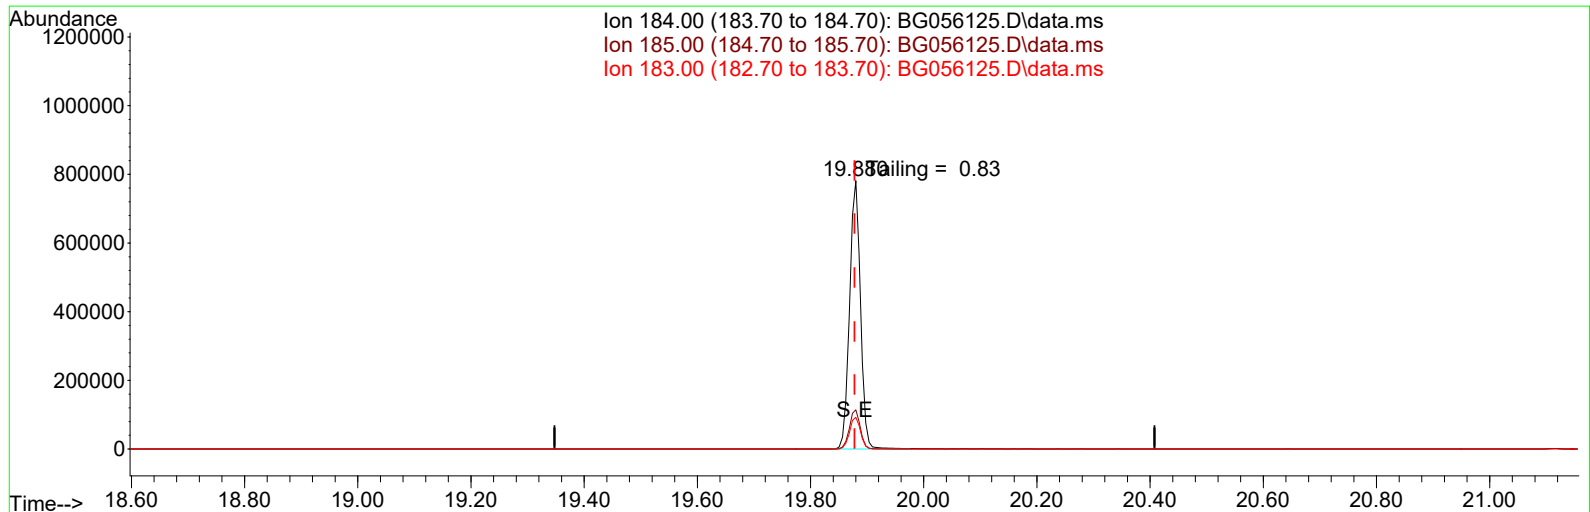

TIC: BG056125.D\data.ms

(77) Benzidine**19.880min (+ 0.002) 489409.95 ng****response 1046213**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.63
183.00	11.70	11.80
0.00	0.00	0.00