
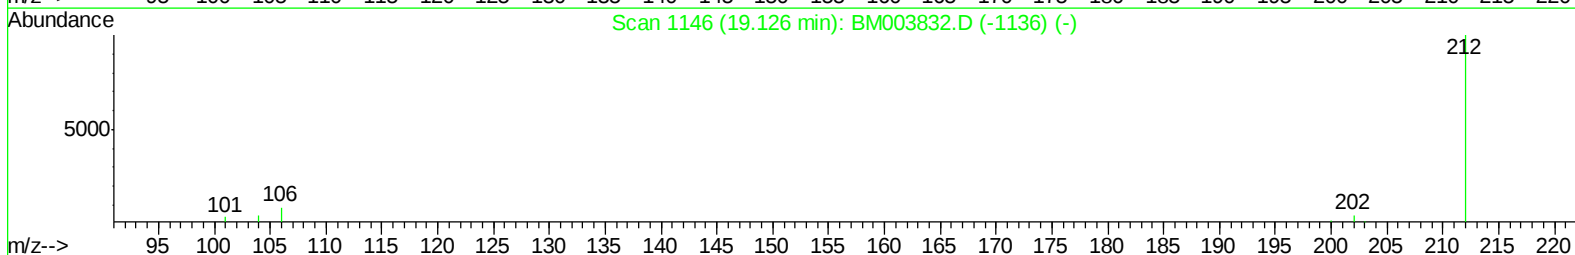
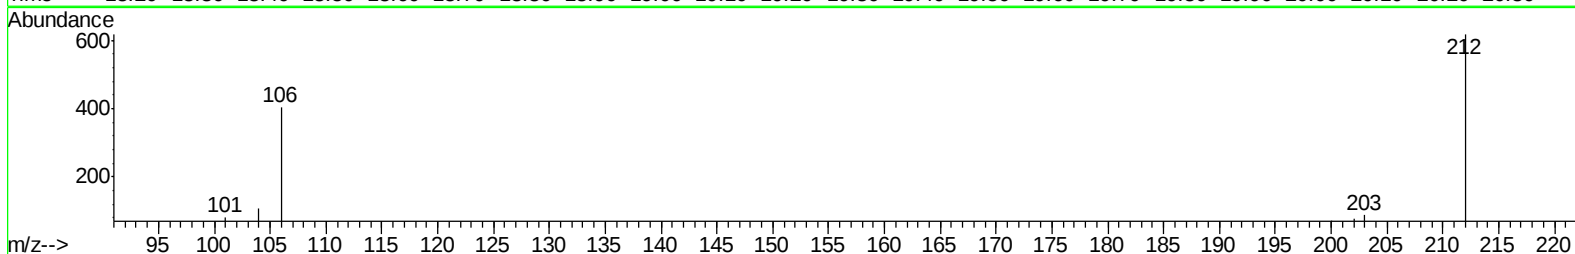


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM123015\
Data File : BM003833.D
Acq On : 28 Dec 2015 17:58
Operator : SJ/UM
Sample : PB87376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 29 07:18:12 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 29 07:09:39 2015
Response via : Initial Calibration

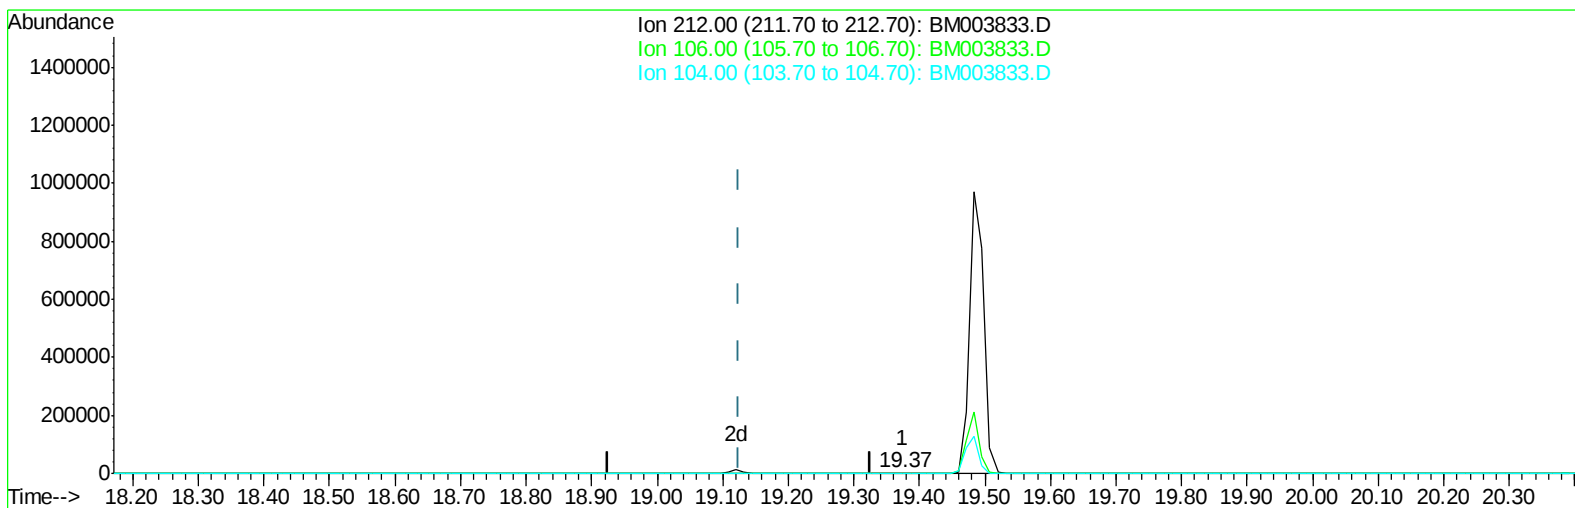

TIC: BM003833.D

(16) Fluoranthene-d10 (SURR)

19.375min (+0.249) 0.02ng/ul

response 733

Ion	Exp%	Act%
212.00	100	100
106.00	18.90	79.54#
104.00	11.10	7.78#
0.00	0.00	0.00