
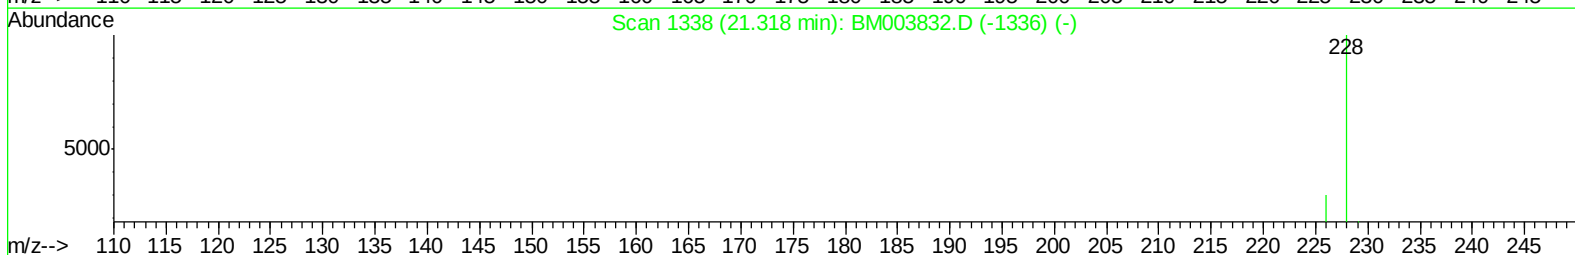
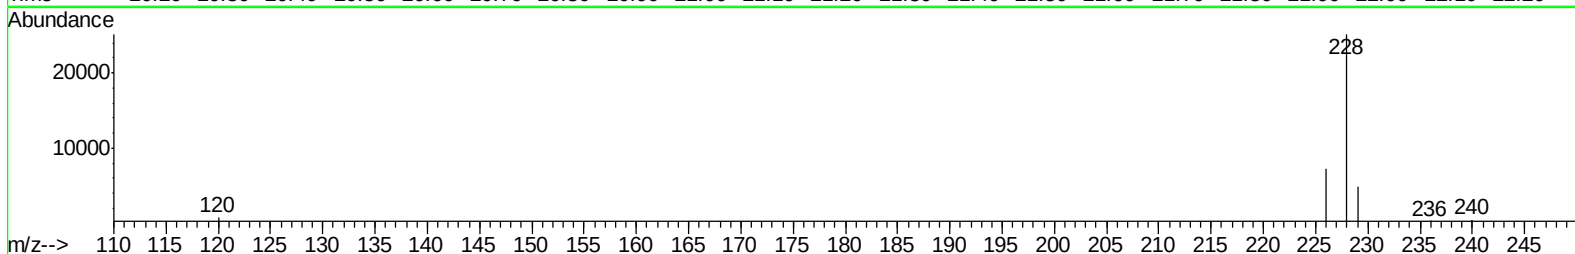


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM123015\
 Data File : BM003838.D
 Acq On : 28 Dec 2015 20:58
 Operator : SJ/UM
 Sample : G4849-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 29 07:42:39 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 29 07:09:39 2015
 Response via : Initial Calibration

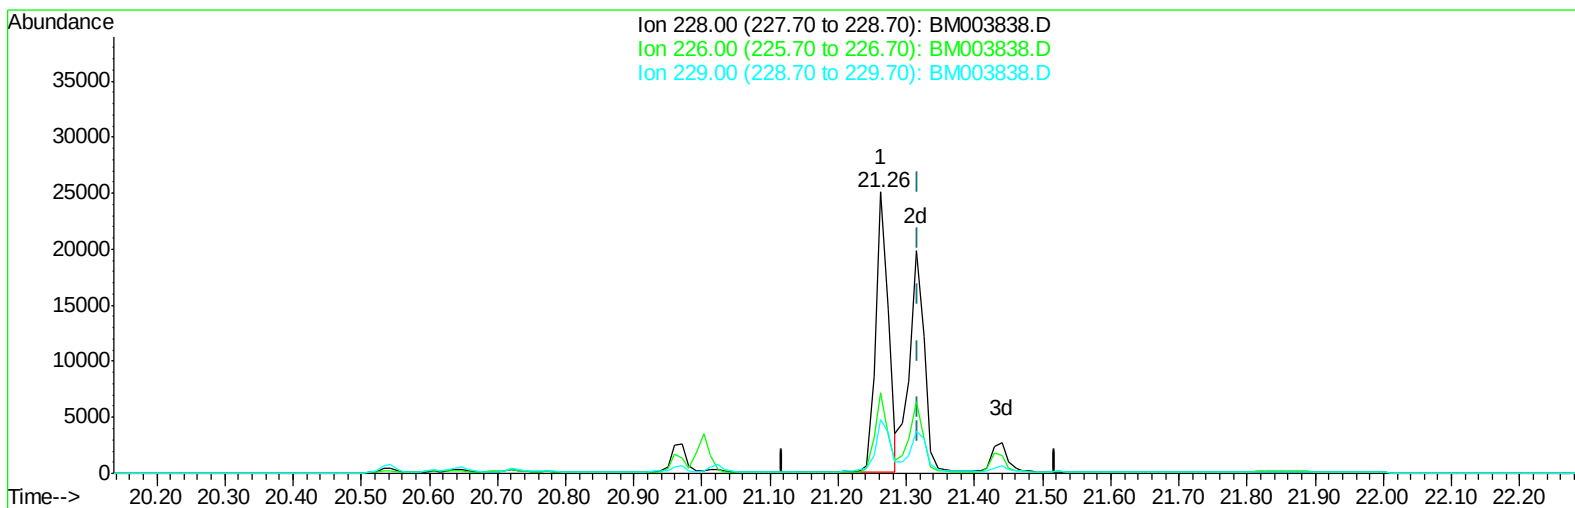

TIC: BM003838.D

(21) Chrysene

21.263min (-0.055) 0.64ng/ul

response 32721

Ion	Exp%	Act%
228.00	100	100
226.00	26.50	28.70
229.00	21.30	19.30
0.00	0.00	0.00