
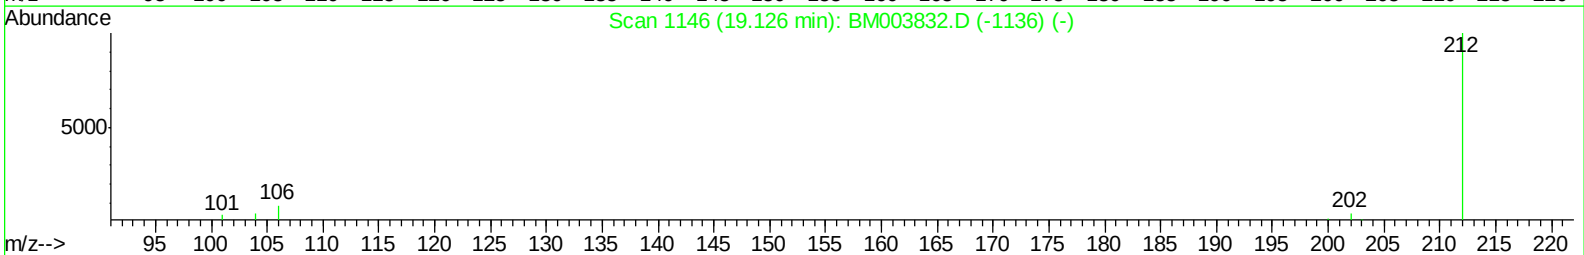
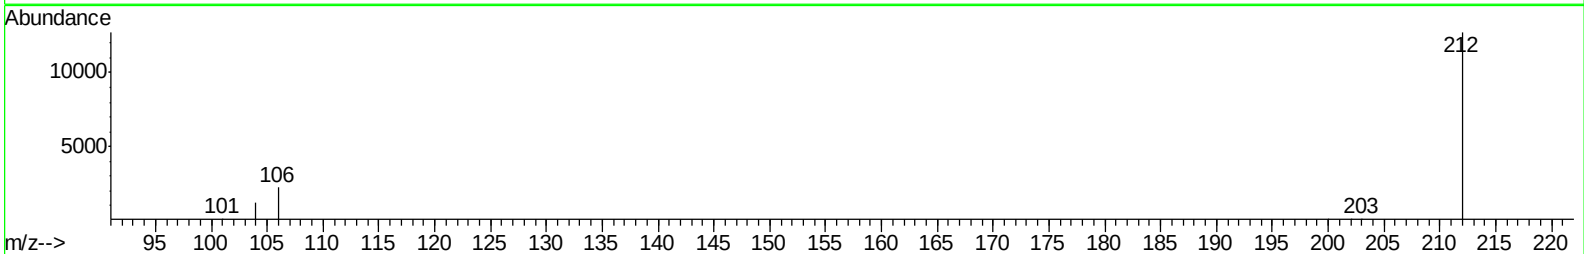


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM123015\
Data File : BM003840.D
Acq On : 28 Dec 2015 22:09
Operator : SJ/UM
Sample : G4849-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 29 07:57:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 29 07:09:39 2015
Response via : Initial Calibration

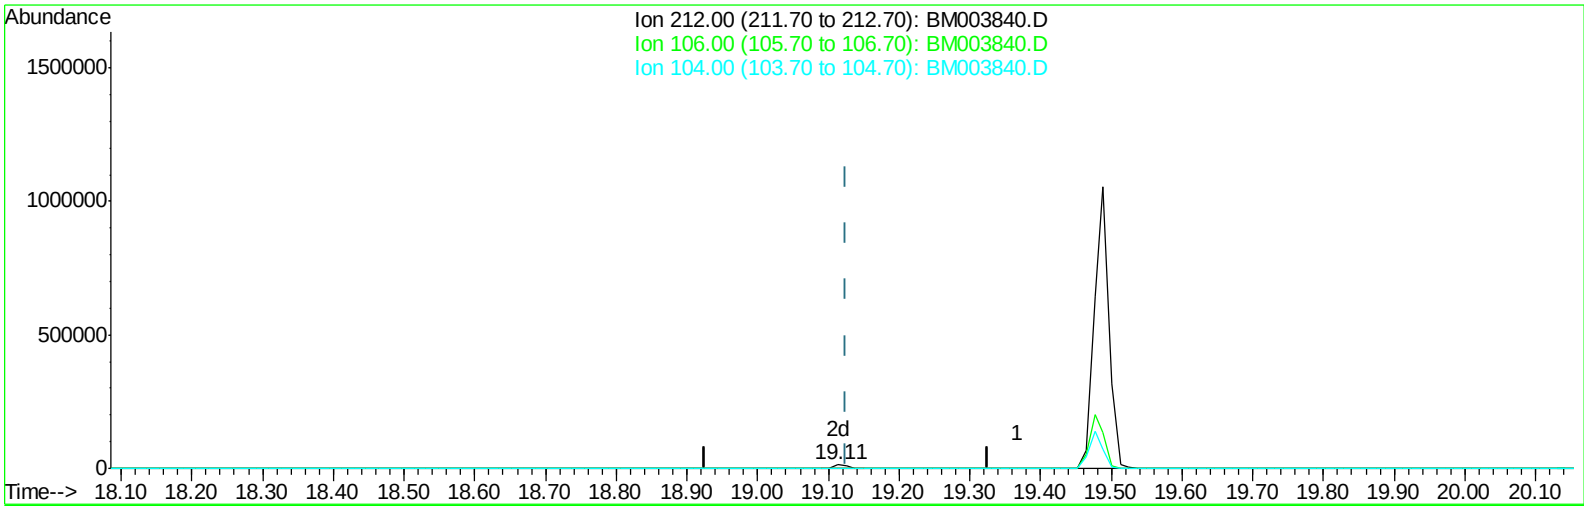

TIC: BM003840.D

(16) Fluoranthene-d10 (SURRE)

19.113min (-0.012) 0.44ng/ul m

response 19580

Ion	Exp%	Act%
212.00	100	100
106.00	18.90	3.19#
104.00	11.10	0.00#
0.00	0.00	0.00