
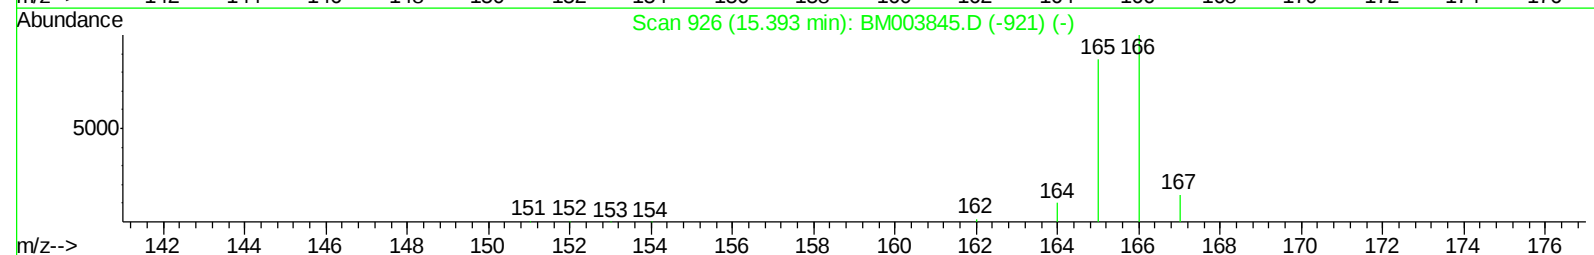
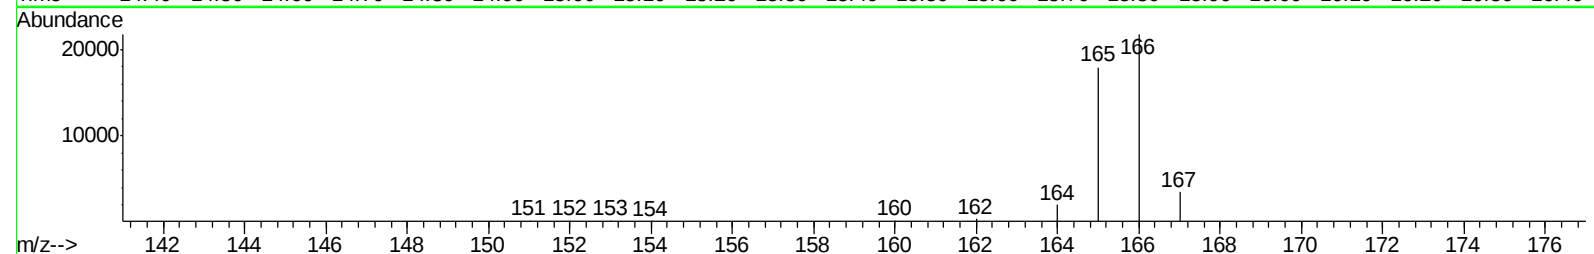


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM123015\
Data File : BM003848.D
Acq On : 29 Dec 2015 03:31
Operator : SJ/UM
Sample : G4848-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 29 08:22:11 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 29 08:19:02 2015
Response via : Initial Calibration

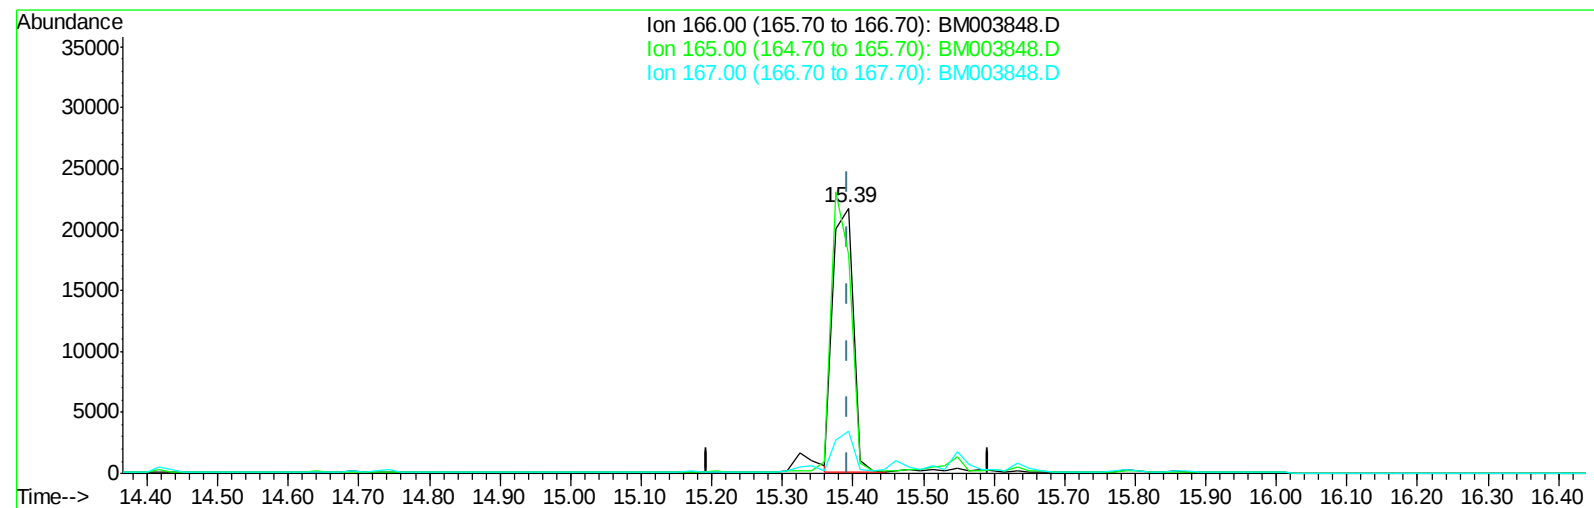

TIC: BM003848.D

(11) Fluorene

15.393min (+0.000) 1.15ng/ul m

response 44082

Ion	Exp%	Act%
166.00	100	100
165.00	87.00	82.36
167.00	14.90	15.76
0.00	0.00	0.00