

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122815\
 Data File : BG020568.D
 Acq On : 28 Dec 2015 17:16
 Operator : UM/SJ
 Sample : G4846-11DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N57DL

Quant Time: Dec 29 03:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 29 02:56:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	12848	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	54024	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	43237	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	133336	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	168027	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	162317	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.23	99	1364	1.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	3705	6.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	4145	5.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.78	113	2838	3.27	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	2517	5.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	3012	6.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.51	165	5318	5.71	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.10	166	26274	7.37	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	27766	6.73	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.69	176	24037	7.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	2511	2.84	ng/ul	0.00
71) Anthracene-d10	17.55	188	43221	6.92	ng/ul	0.00
79) Pyrene-d10	19.84	212	54458	7.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	56207	6.85	ng/ul	0.00

Target Compounds


						Ovalue
28) Naphthalene	10.93	128	78018	27.17	ng/ul	98
34) 2-Methylnaphthalene	12.54	142	12099	5.69	ng/ul	93
41) 1,1'-Biphenyl	13.54	154	4254	1.27	ng/ul	94
50) Acenaphthene	14.77	153	22571	7.69	ng/ul	96
54) Dibenzofuran	15.10	168	16613	3.81	ng/ul	100
59) Fluorene	15.75	166	15425	4.36	ng/ul	98
70) Phenanthrene	17.49	178	41518	5.60	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122815\
Data File : BG020568.D
Acq On : 28 Dec 2015 17:16
Operator : UM/SJ
Sample : G4846-11DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N57DL

Quant Time: Dec 29 03:07:21 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 29 02:56:07 2015
Response via : Initial Calibration

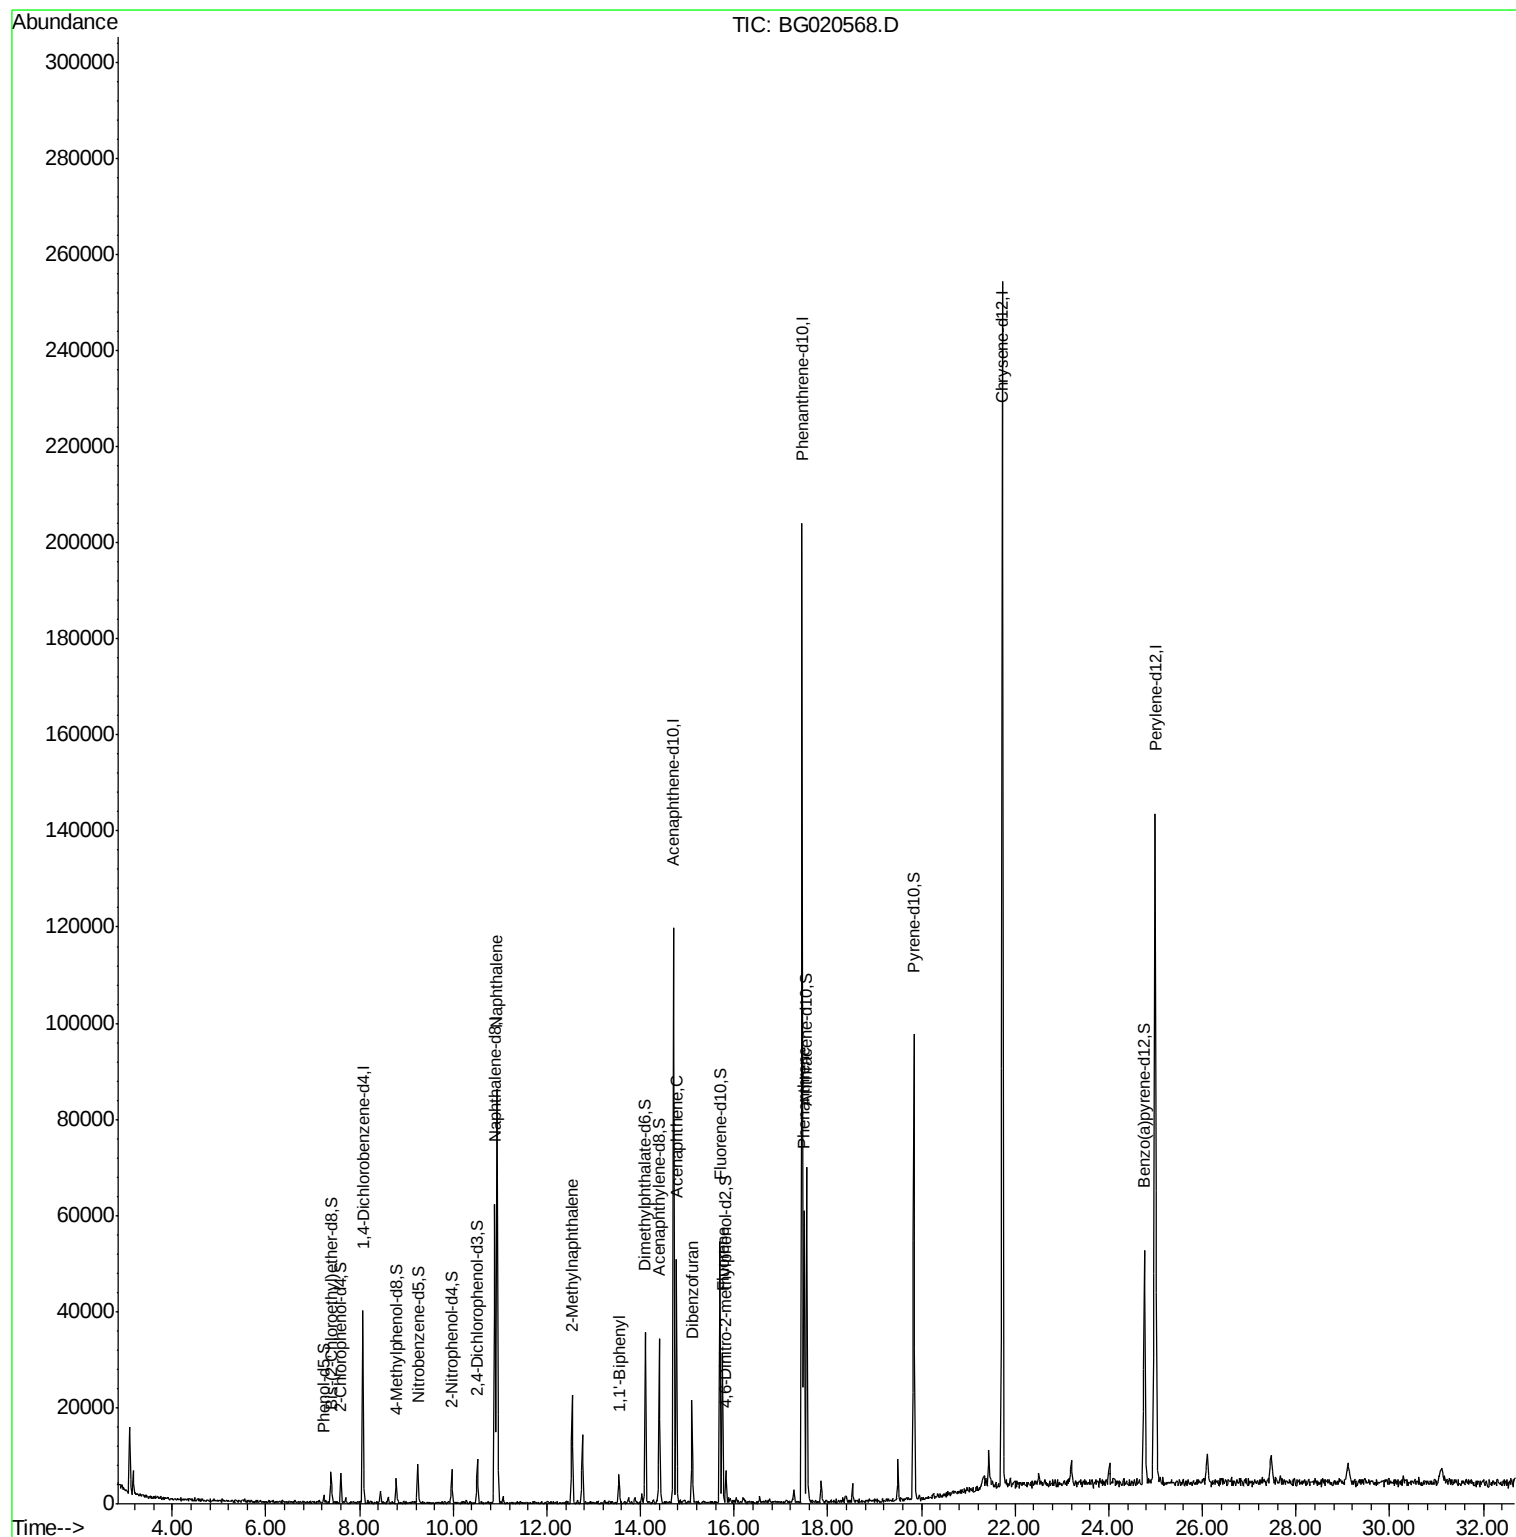


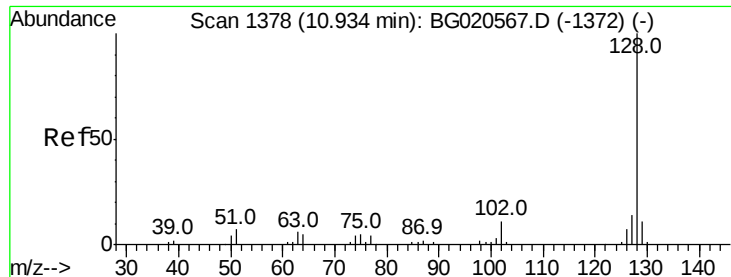




#28
Naphthalene
Concen: 27.17 ng/ul
RT: 10.93 min Scan# 1378
Delta R.T. 0.00 min
Lab File: BG020568.D
Acq: 28 Dec 2015 17:16

Instrument :
BNA_G
ClientSampleId :
D9N57DL

Tot Ion:128 Resp: 78018
Ion Ratio Lower Upper
128 100
129 10.4 8.6 12.8
127 13.9 10.1 15.1

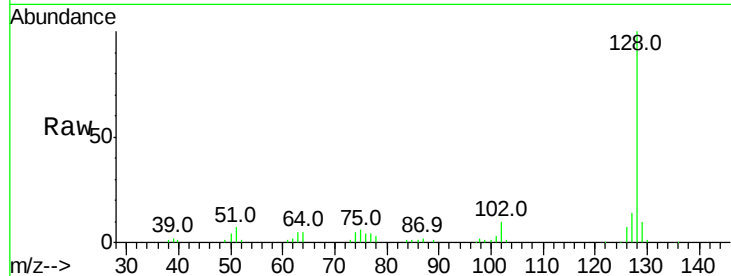


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

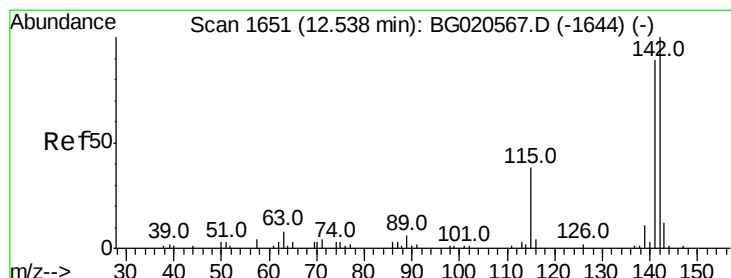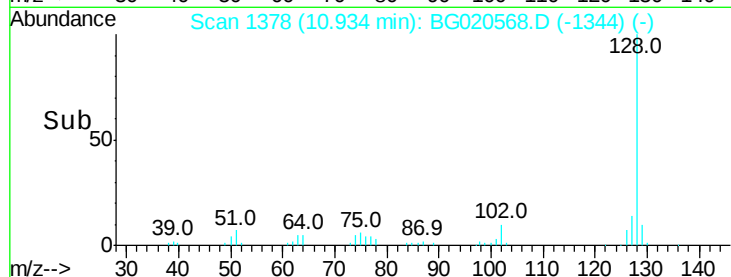
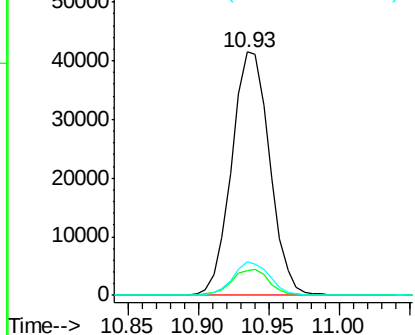



#34
2-Methylnaphthalene
Concen: 5.69 ng/ul
RT: 12.54 min Scan# 1651
Delta R.T. 0.00 min
Lab File: BG020568.D
Acq: 28 Dec 2015 17:16

Tgt Ion:142 Resp: 12099
Ion Ratio Lower Upper
142 100
141 87.1 74.9 112.3

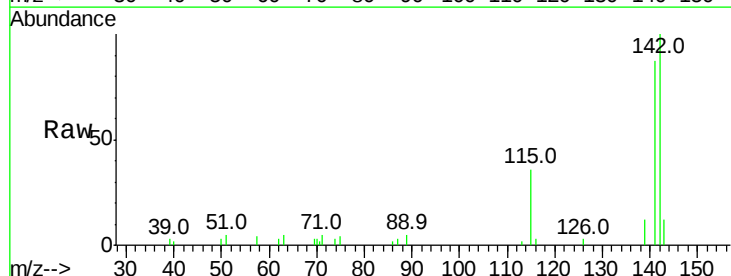

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

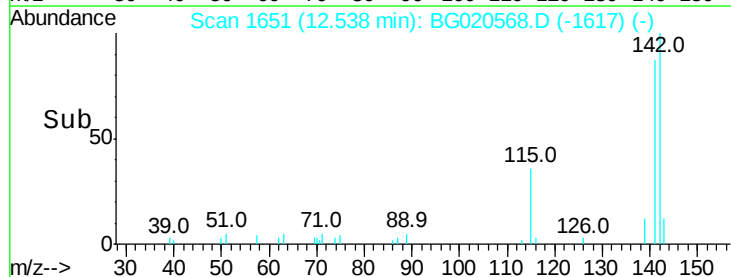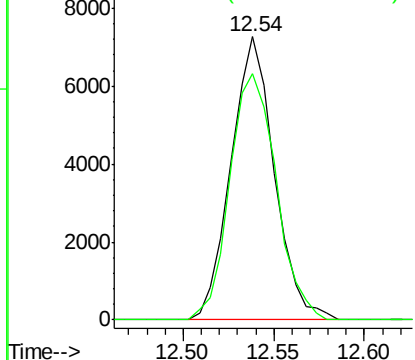


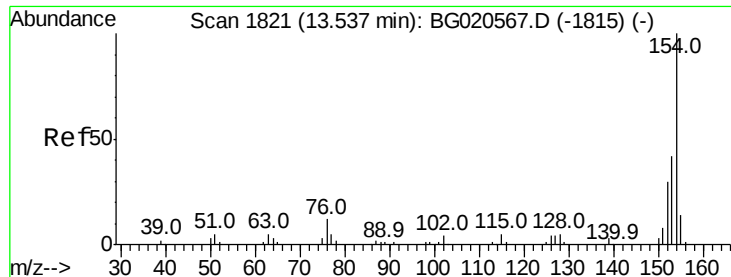




#41
 1,1'-Biphenyl
 Concen: 1.27 ng/ul
 RT: 13.54 min Scan# 1822
 Delta R.T. 0.01 min
 Lab File: BG020568.D
 Acq: 28 Dec 2015 17:16

Instrument :
 BNA_G
 ClientSampleId :
 D9N57DL

Tot Ion	Ratio	Lower	Upper
154	100		
153	39.4	35.5	53.3
76	12.6	10.4	15.6

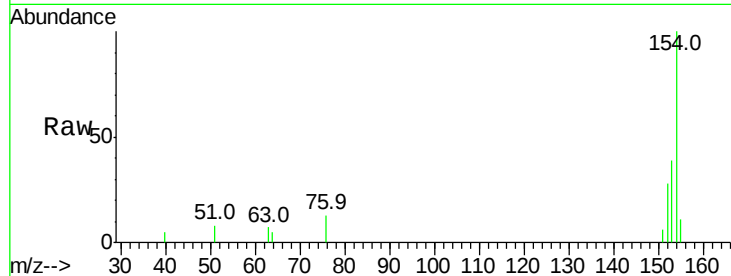


Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): B

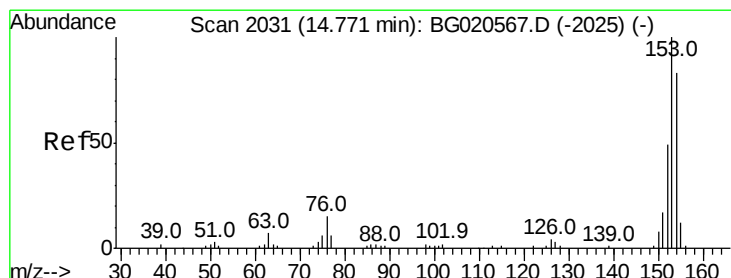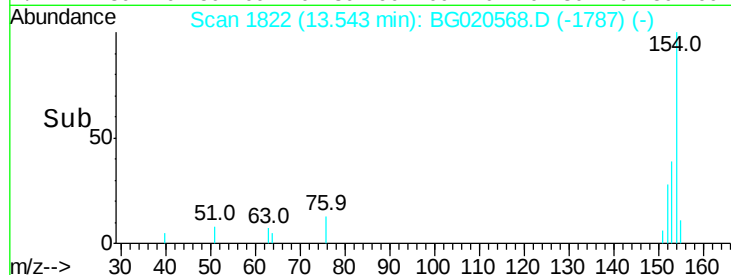
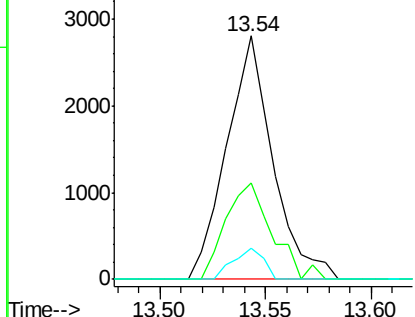



#50
 Acenaphthene
 Concen: 7.69 ng/ul
 RT: 14.77 min Scan# 2031
 Delta R.T. 0.00 min
 Lab File: BG020568.D
 Acq: 28 Dec 2015 17:16

Tgt Ion	Ratio	Lower	Upper
153	100		
152	50.2	37.6	56.4
154	87.5	67.9	101.9

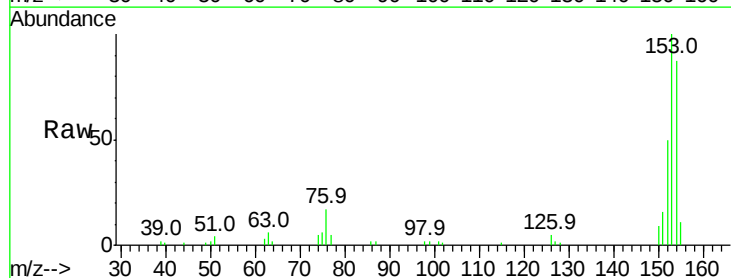

Abundance Ion 153.00 (152.70 to 153.70): E
 Ion 152.00 (151.70 to 152.70): E
 Ion 154.00 (153.70 to 154.70): E

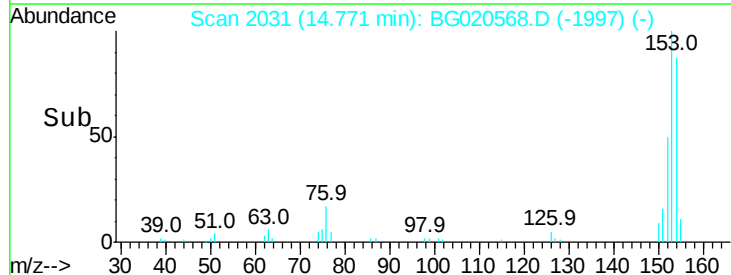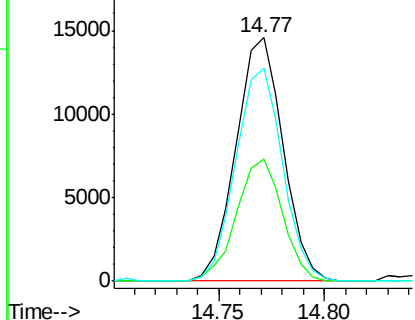

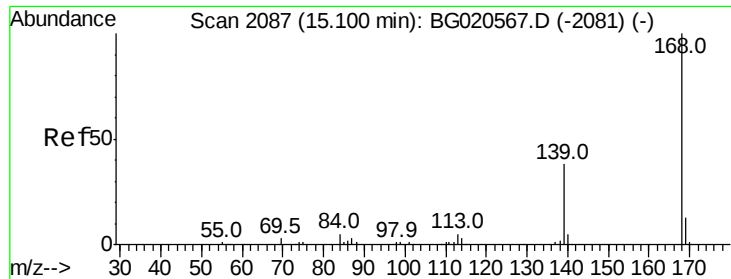

#54

Dibenzenofuran

Concen: 3.81 ng/ul

RT: 15.10 min Scan# 2087

Delta R.T. 0.00 min

Lab File: BG020568.D

Acq: 28 Dec 2015 17:16

Instrument :

BNA_G

ClientSampleId :


D9N57DL

Tot Ion:168 Resp: 16613

Ion Ratio Lower Upper

168 100

139 38.0 30.5 45.7

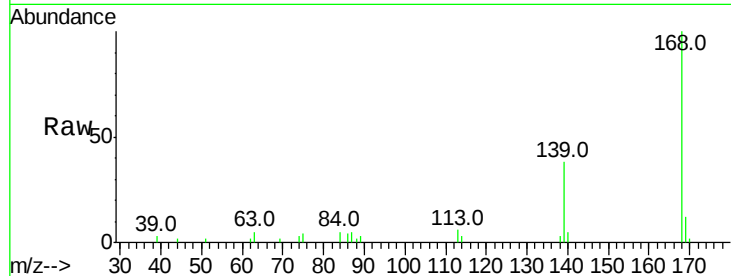

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

12000

10000

8000

6000

4000

2000



0

15.05

15.10

15.15

Time-->

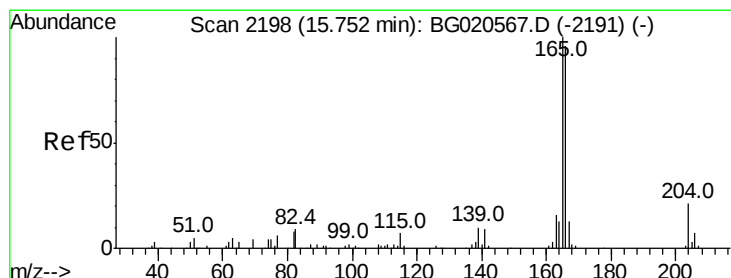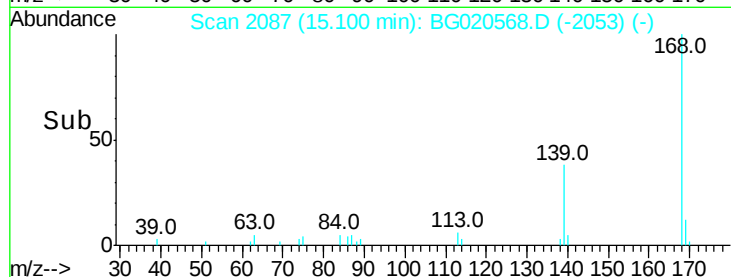

#59

Fluorene

Concen: 4.36 ng/ul

RT: 15.75 min Scan# 2198

Delta R.T. 0.00 min

Lab File: BG020568.D

Acq: 28 Dec 2015 17:16


Tgt Ion:166 Resp: 15425

Ion Ratio Lower Upper

166 100

165 100.0 81.4 122.0

167 15.0 11.2 16.8

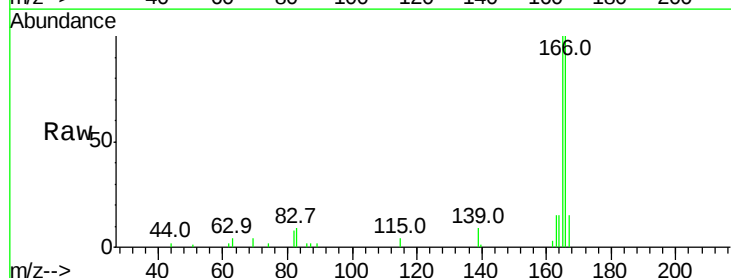

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

10000

5000


0


15.70

15.75

15.80

Time-->

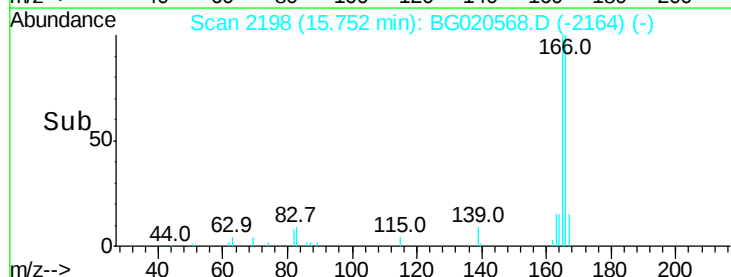

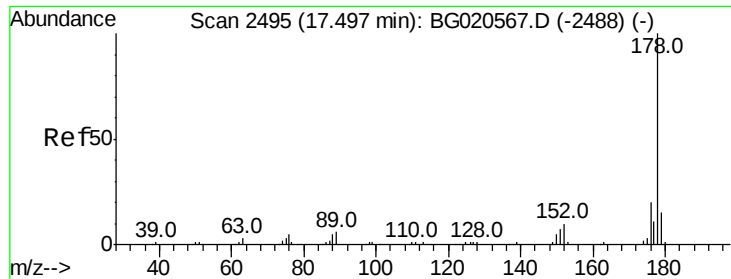

#70

Phenanthrene

Concen: 5.60 ng/ul

RT: 17.49 min Scan# 2494

Delta R.T. -0.01 min

Lab File: BG020568.D

Acq: 28 Dec 2015 17:16

Instrument :

BNA_G

ClientSampleId :

D9N57DL


Tot Ion:178 Resp: 41518

Ion Ratio Lower Upper

178 100

179 16.1 12.9 19.3

176 20.5 15.3 22.9

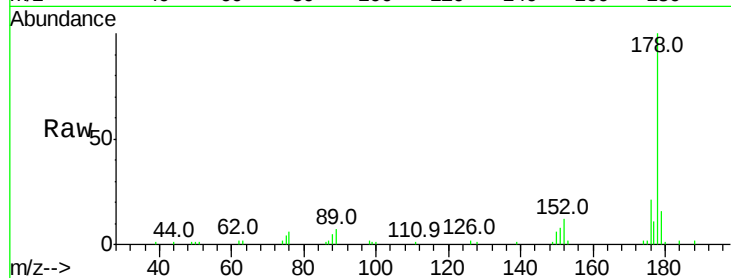

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

