

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122815\
 Data File : BG020579.D
 Acq On : 29 Dec 2015 1:04
 Operator : UM/SJ
 Sample : G4847-02DL 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleID :
 D9N68DL

Manual Integrations
 APPROVED

UMANGI
 12/29/2015 4:55:08 PM

Quant Time: Dec 29 06:04:20 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 29 05:04:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	12278	20.00	ng/ul	0.00
18) Naphthalene-d8	10.89	136	54056	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.70	164	43389	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	135861	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	186252	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	175803	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	7.39	67	1492	2.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	1779	2.35	ng/ul	0.01
13) 4-Methylphenol-d8	8.78	113	928m	1.12	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	1133	2.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	1253	2.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	2220	2.38	ng/ul	0.01
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.10	166	12785	3.57	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	13781	3.33	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.69	176	12040	3.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	17.55	188	23308	3.66	ng/ul	0.00
79) Pyrene-d10	19.84	212	28242	3.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	28106	3.16	ng/ul	-0.01

Target Compounds

						Ovalue
28) Naphthalene	10.93	128	117069	40.74	ng/ul	99
34) 2-Methylnaphthalene	12.54	142	12686	5.97	ng/ul	93
50) Acenaphthene	14.77	153	12606	4.28	ng/ul	96
54) Dibenzofuran	15.10	168	9560	2.18	ng/ul	91
59) Fluorene	15.75	166	8039	2.26	ng/ul#	95
70) Phenanthrene	17.49	178	17499	2.31	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122815\
Data File : BG020579.D
Acq On : 29 Dec 2015 1:04
Operator : UM/SJ
Sample : G4847-02DL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
D9N68DL

Manual Integrations
APPROVED

UMANGI
12/29/2015 4:55:08 PM

Quant Time: Dec 29 06:04:20 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG122415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 29 05:04:12 2015
Response via : Initial Calibration

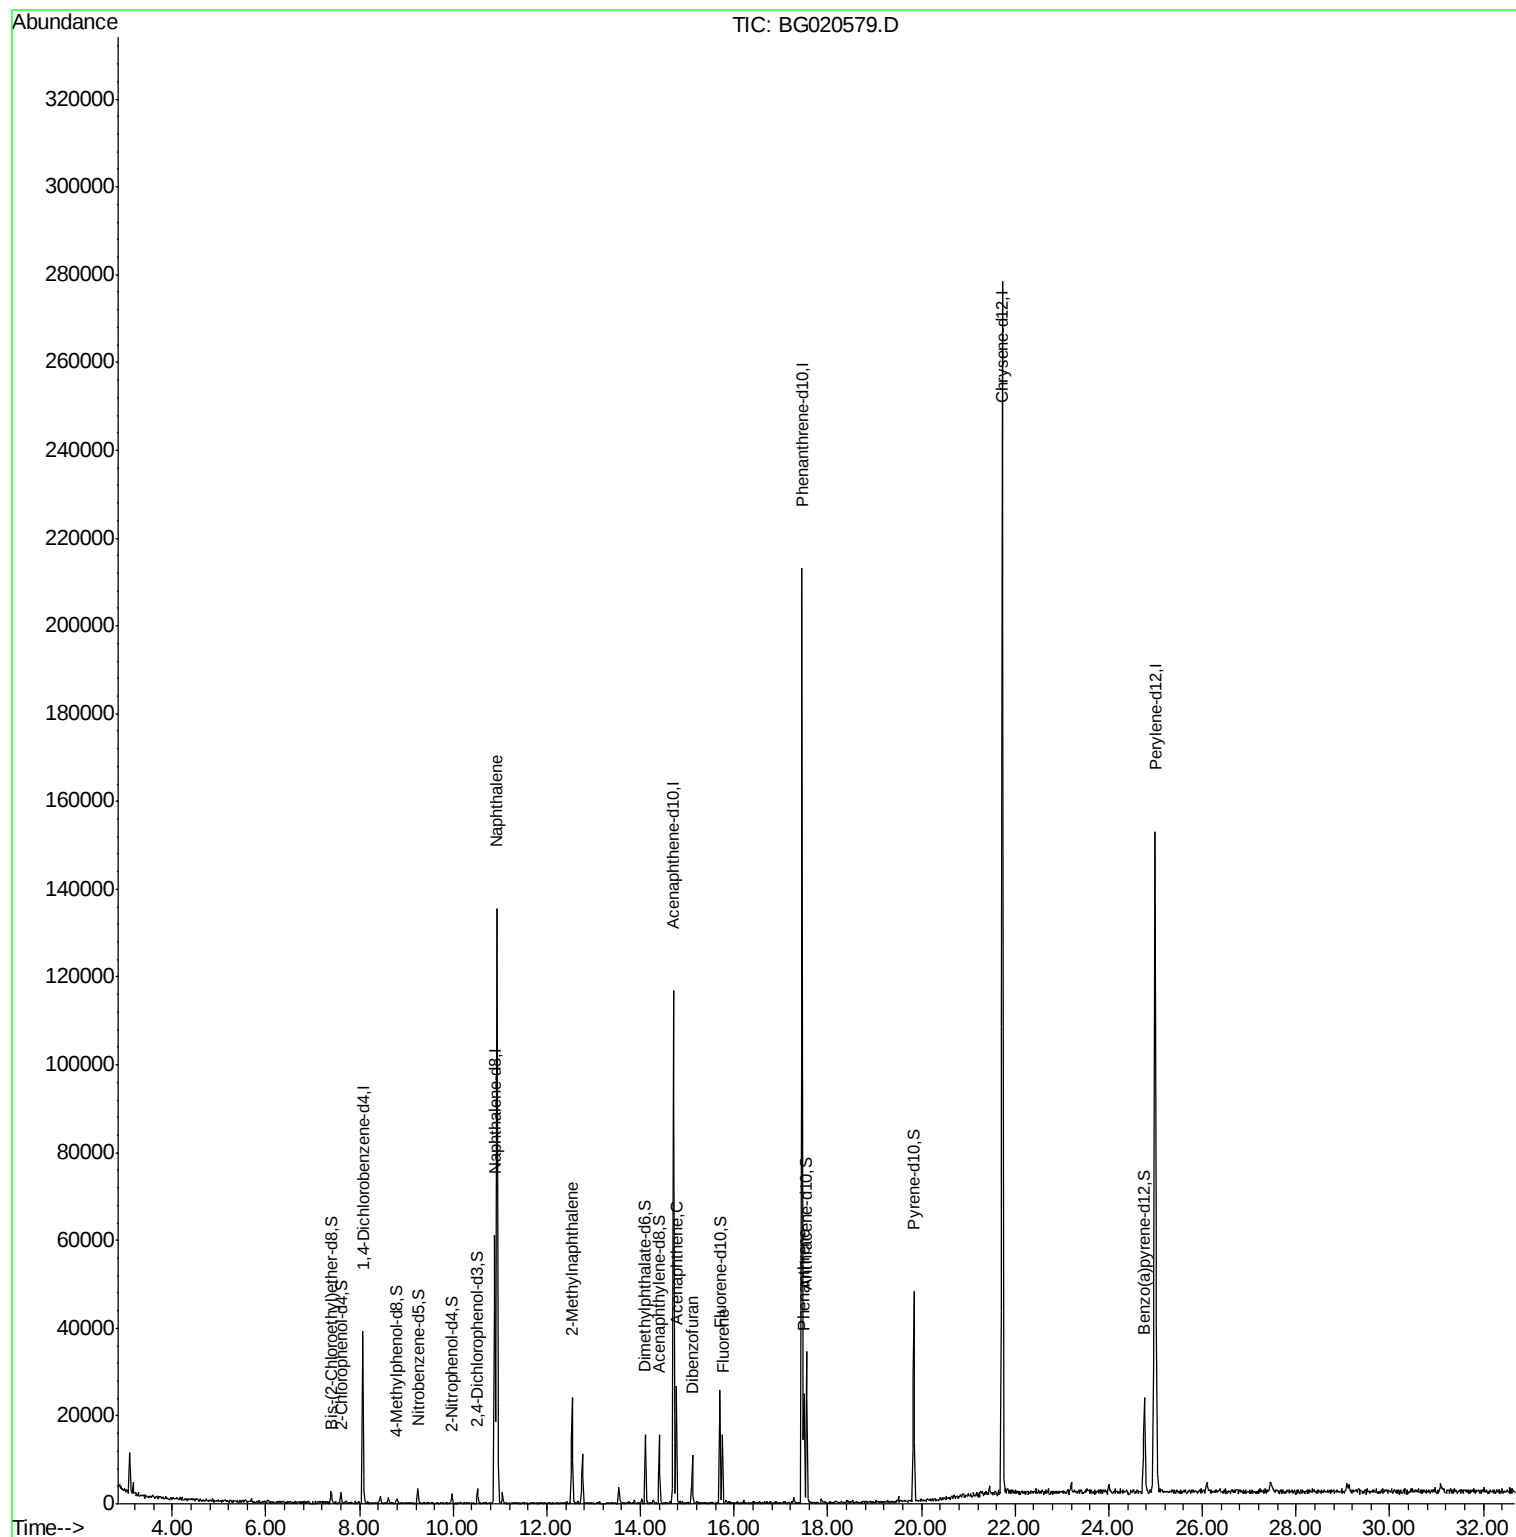

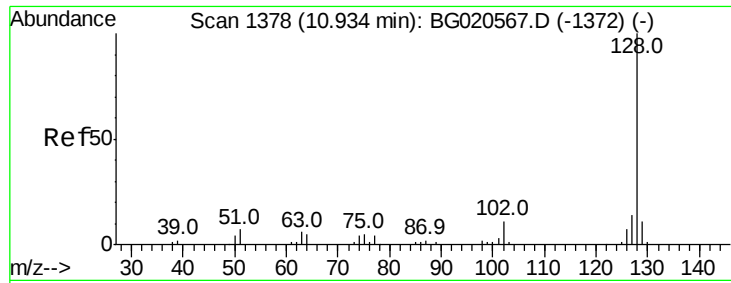





#28
Naphthalene
Concen: 40.74 ng/ul
RT: 10.93 min Scan# 1378
Delta R.T. 0.00 min
Lab File: BG020579.D
Acq: 29 Dec 2015 1:04

Instrument :
BNA_G
ClientSampleId :
D9N68DL

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.2	8.6	12.8
127	13.0	10.1	15.1




Manual Integrations
APPROVED


UMANGI
12/29/2015 4:55:08 PM

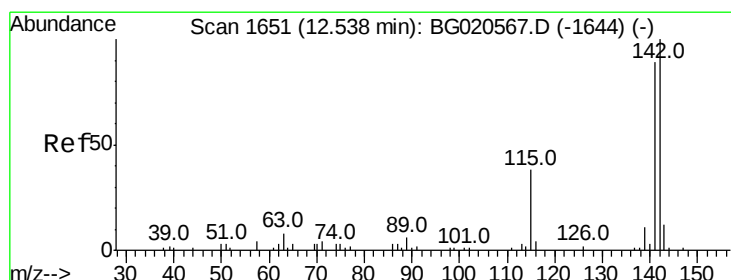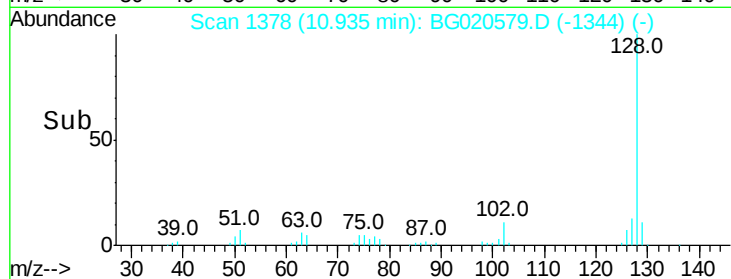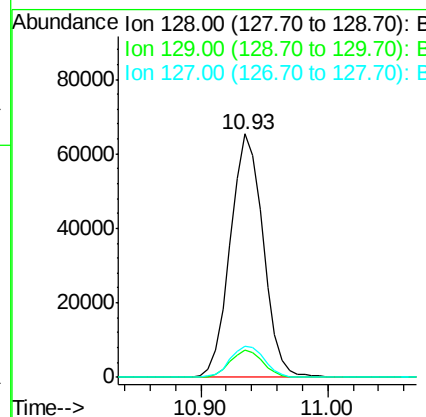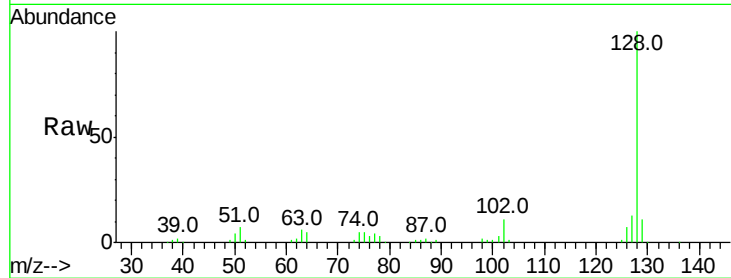

#34
2-Methylnaphthalene
Concen: 5.97 ng/ul
RT: 12.54 min Scan# 1651
Delta R.T. 0.00 min
Lab File: BG020579.D
Acq: 29 Dec 2015 1:04

Tgt Ion	Ratio	Lower	Upper
142	100		
141	86.6	74.9	112.3

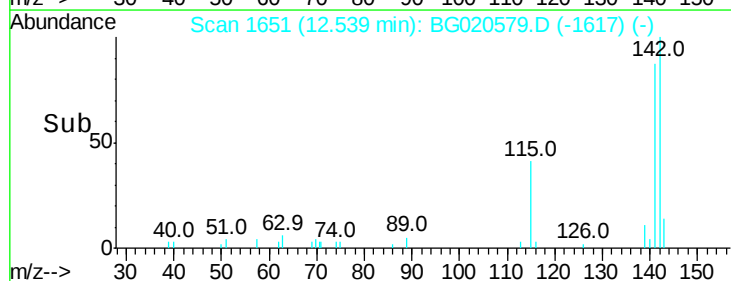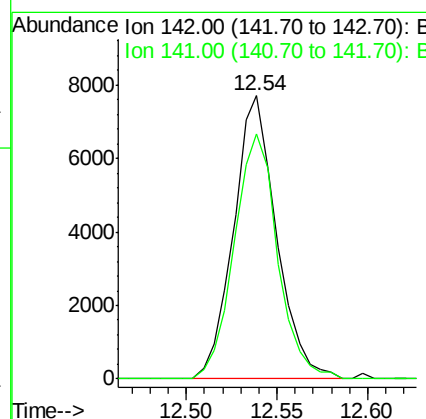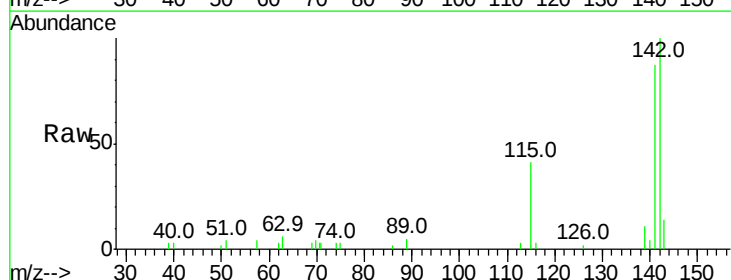

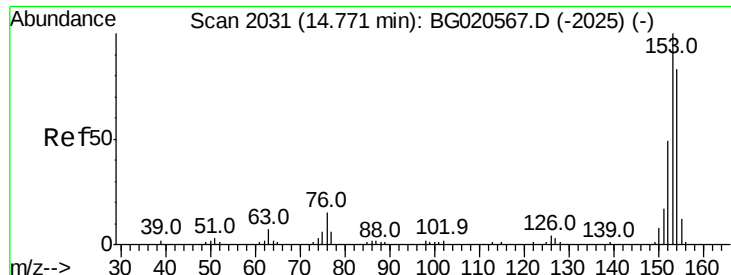


#50
Acenaphthene
Concen: 4.28 ng/ul
RT: 14.77 min Scan# 2030
Delta R.T. 0.00 min
Lab File: BG020579.D
Acq: 29 Dec 2015 1:04

Instrument :
BNA_G
ClientSampleId :
D9N68DL




Tot Ion	Ratio	Lower	Upper
153	100		
152	50.9	37.6	56.4
154	87.3	67.9	101.9

Manual Integrations
APPROVED

UMANGI
12/29/2015 4:55:08 PM

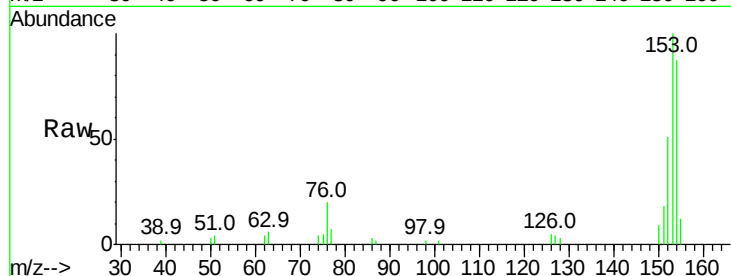


Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

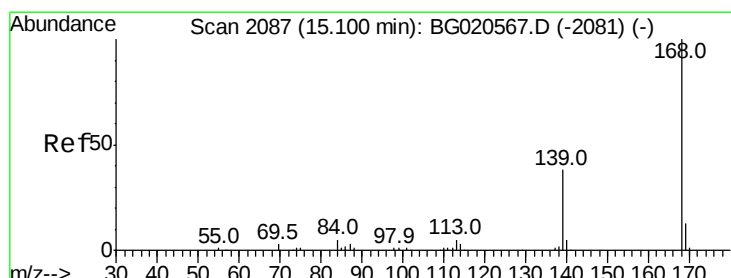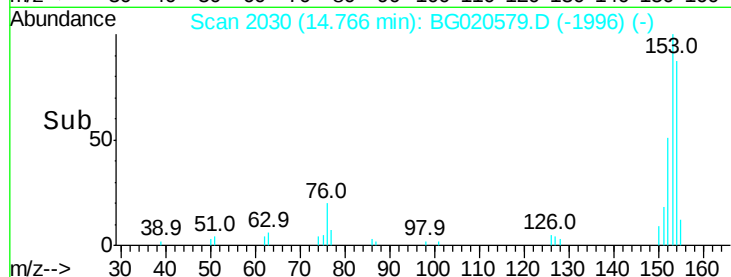
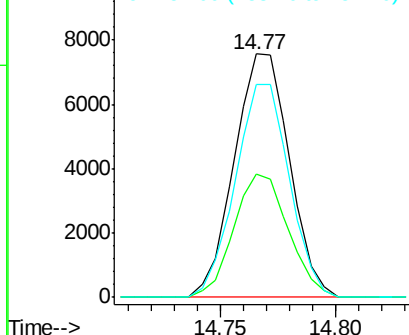



#54
Dibenzofuran
Concen: 2.18 ng/ul
RT: 15.10 min Scan# 2087
Delta R.T. 0.00 min
Lab File: BG020579.D
Acq: 29 Dec 2015 1:04

Tgt Ion	Ratio	Lower	Upper
168	100		
139	32.4	30.5	45.7

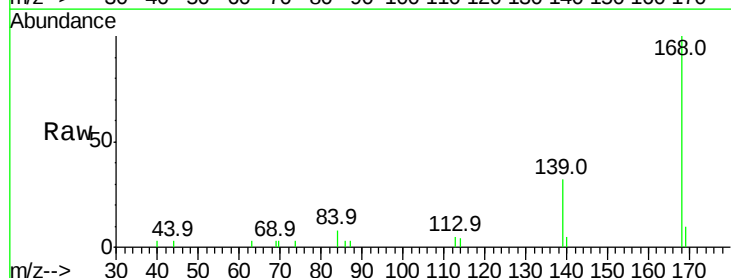

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E

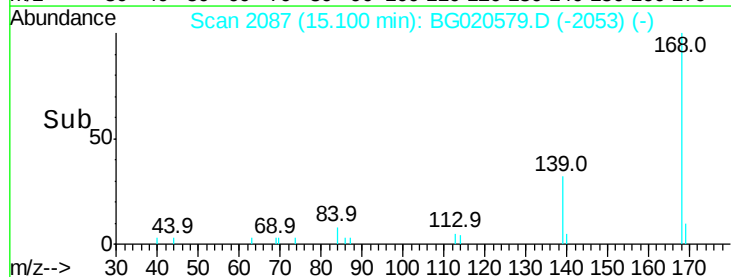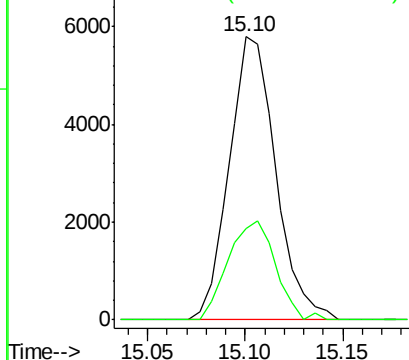

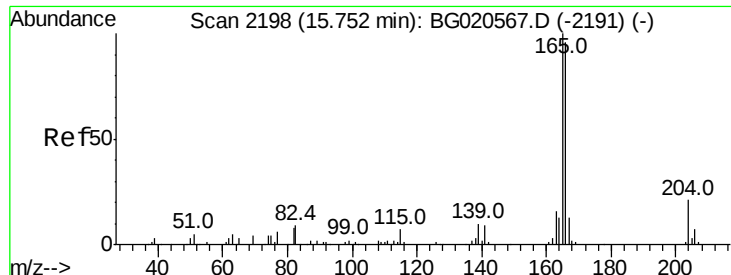





#59
Fluorene
 Concen: 2.26 ng/ul
 RT: 15.75 min Scan# 2198
 Delta R.T. 0.00 min
 Lab File: BG020579.D
 Acq: 29 Dec 2015 1:04

Instrument :
 BNA_G
 ClientSampleId :
 D9N68DL

Tot Ion	Ratio	Resp	Lower	Upper
166	100	8039		
165	97.6		81.4	122.0
167	10.2		11.2	16.8#

Manual Integrations
 APPROVED

UMANGI
 12/29/2015 4:55:08 PM

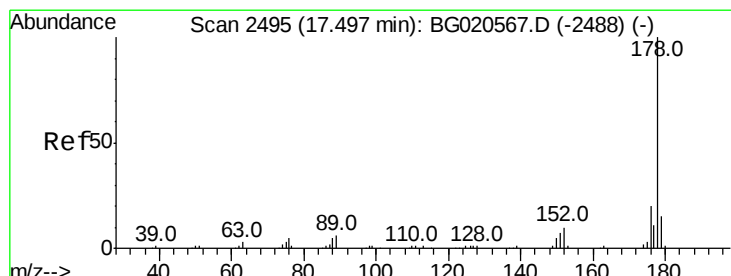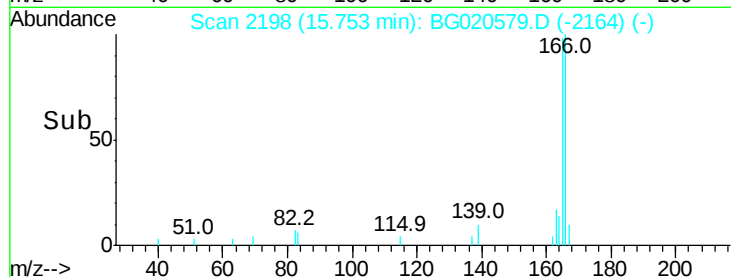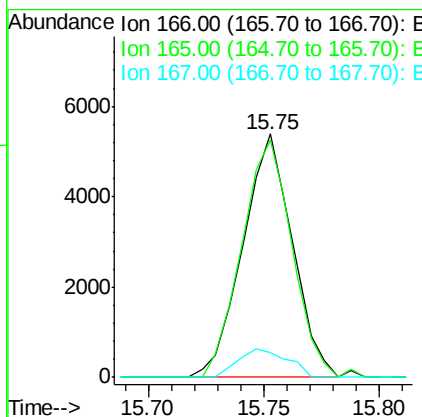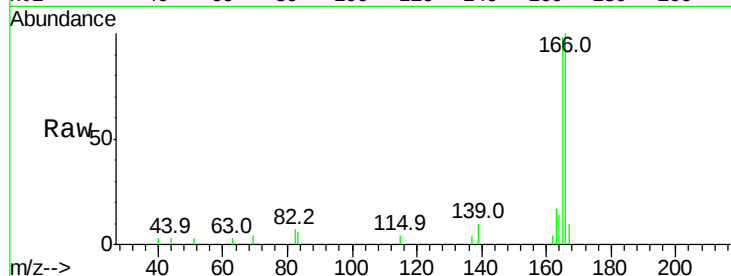

#70
Phenanthrene
 Concen: 2.31 ng/ul
 RT: 17.49 min Scan# 2494
 Delta R.T. 0.00 min
 Lab File: BG020579.D
 Acq: 29 Dec 2015 1:04

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	17499		
179	17.8		12.9	19.3
176	19.4		15.3	22.9

