
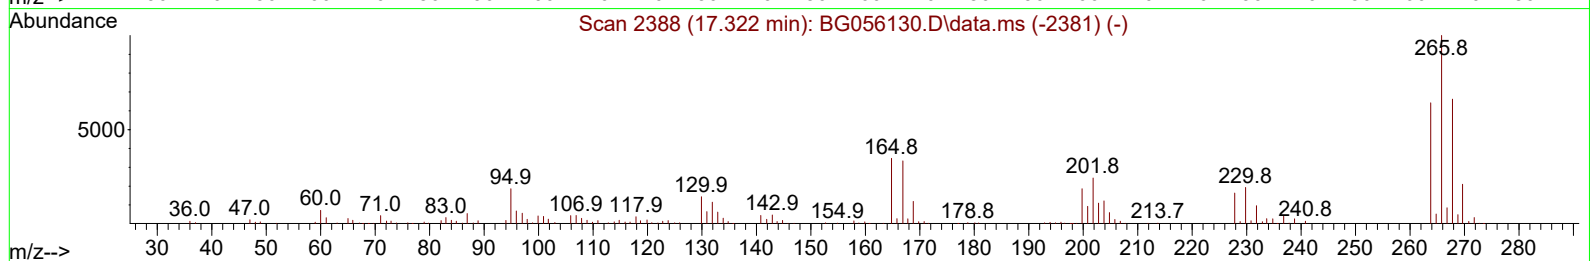
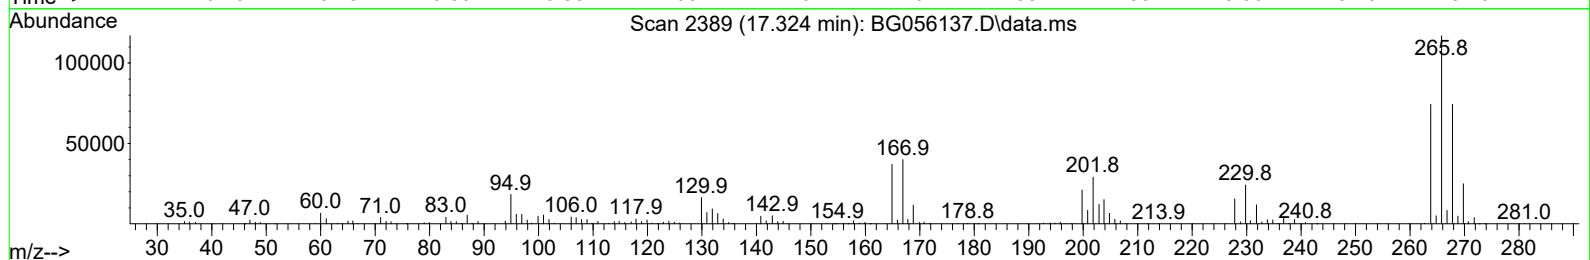


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122822\
Data File : BG056137.D
Acq On : 28 Dec 2022 11:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 04:58:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

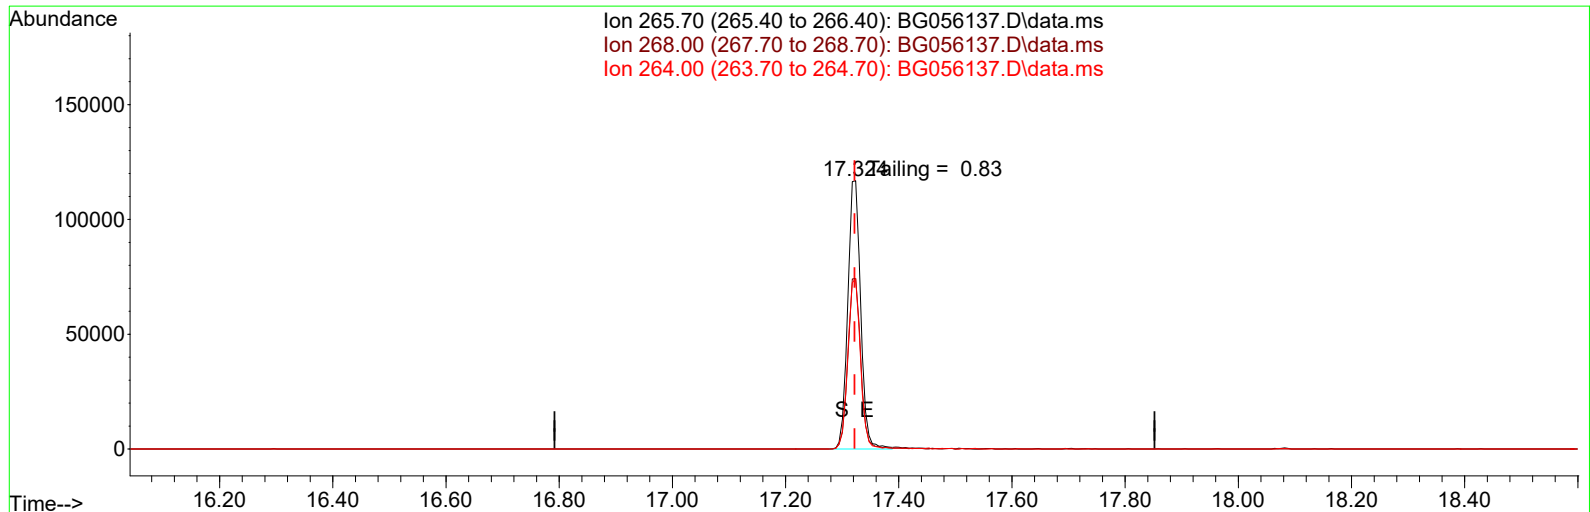

TIC: BG056137.D\data.ms

(70) Pentachlorophenol (C)




17.324min (+ 0.002) 302140.48 ng

response 187504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	63.51
264.00	64.30	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122822\
Data File : BG056137.D
Acq On : 28 Dec 2022 11:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 04:58:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

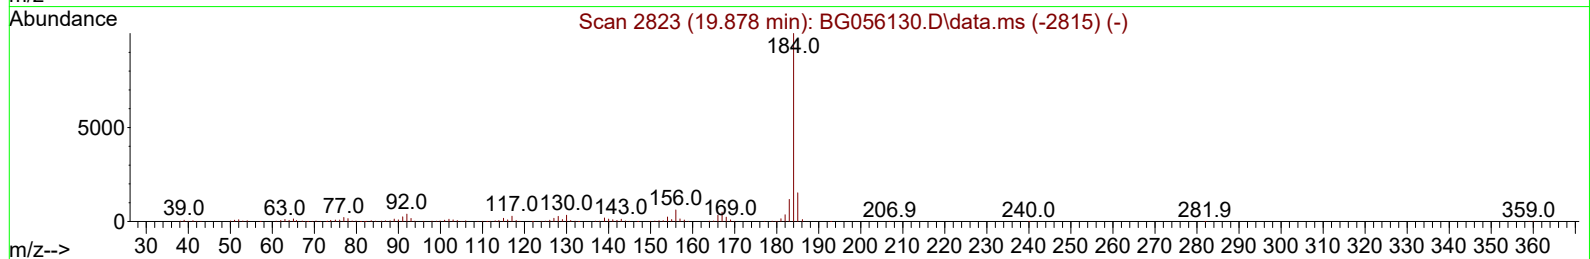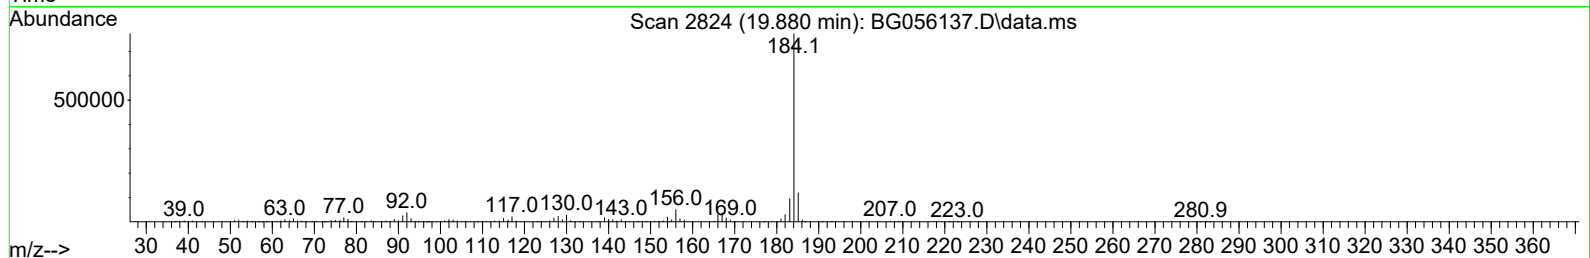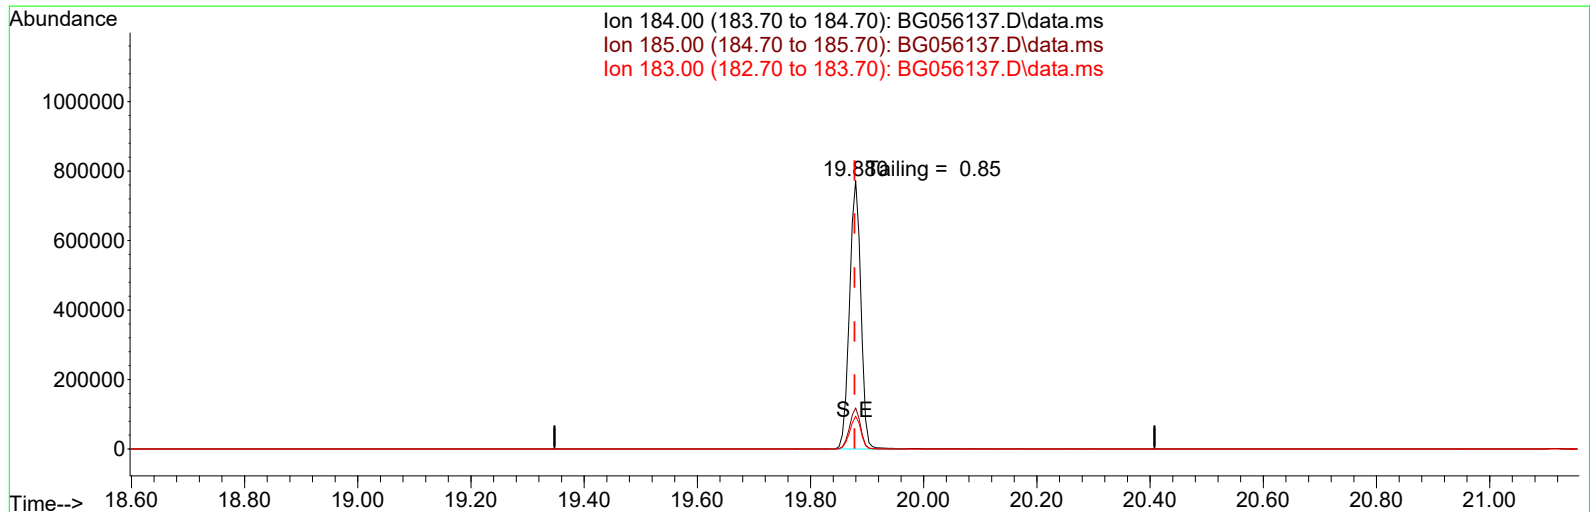

TIC: BG056137.D\data.ms

(77) Benzidine**19.880min (+ 0.002) 393660.62 ng****response 1076054**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.36
183.00	11.70	12.25
0.00	0.00	0.00