
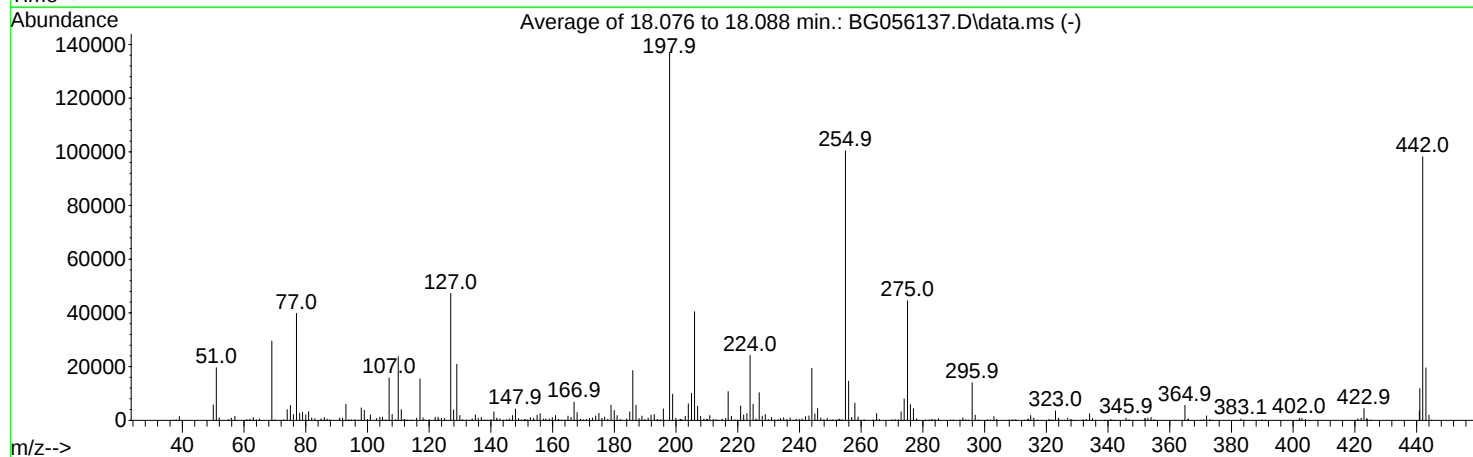


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122822\
 Data File : BG056137.D
 Acq On : 28 Dec 2022 11:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 05:20:14 2022

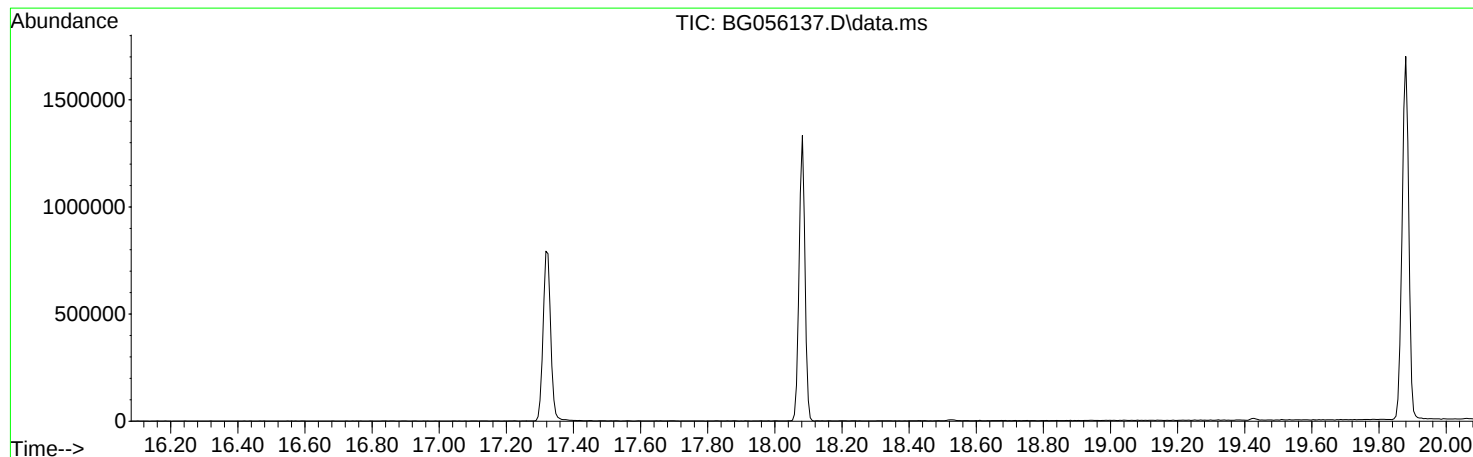




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.3	19560	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.5	29523	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	34.5	47269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137043	PASS
199	198	5	9	7.1	9734	PASS
275	198	10	60	32.5	44573	PASS
365	198	1	100	4.1	5563	PASS
441	198	0.01	100	8.6	11837	PASS
442	442	50	100	100.0	98157	PASS
443	442	15	24	19.9	19504	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122822\
Data File : BG056137.D
Acq On : 28 Dec 2022 11:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 29 04:58:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

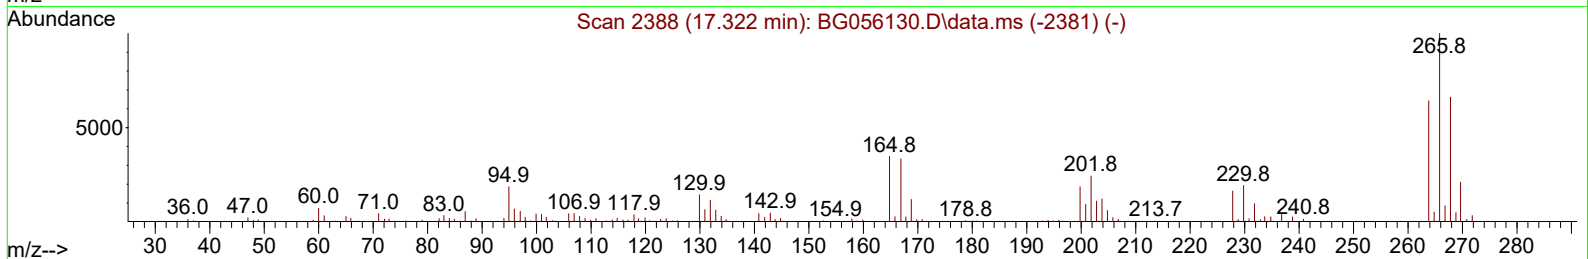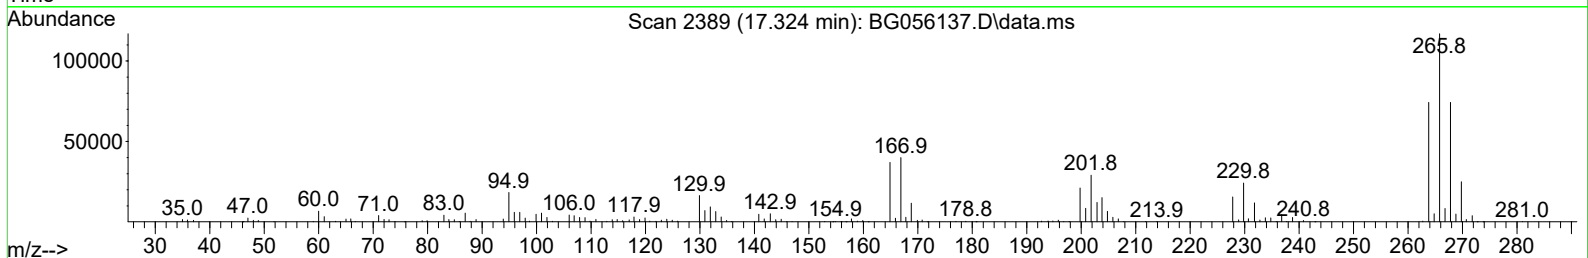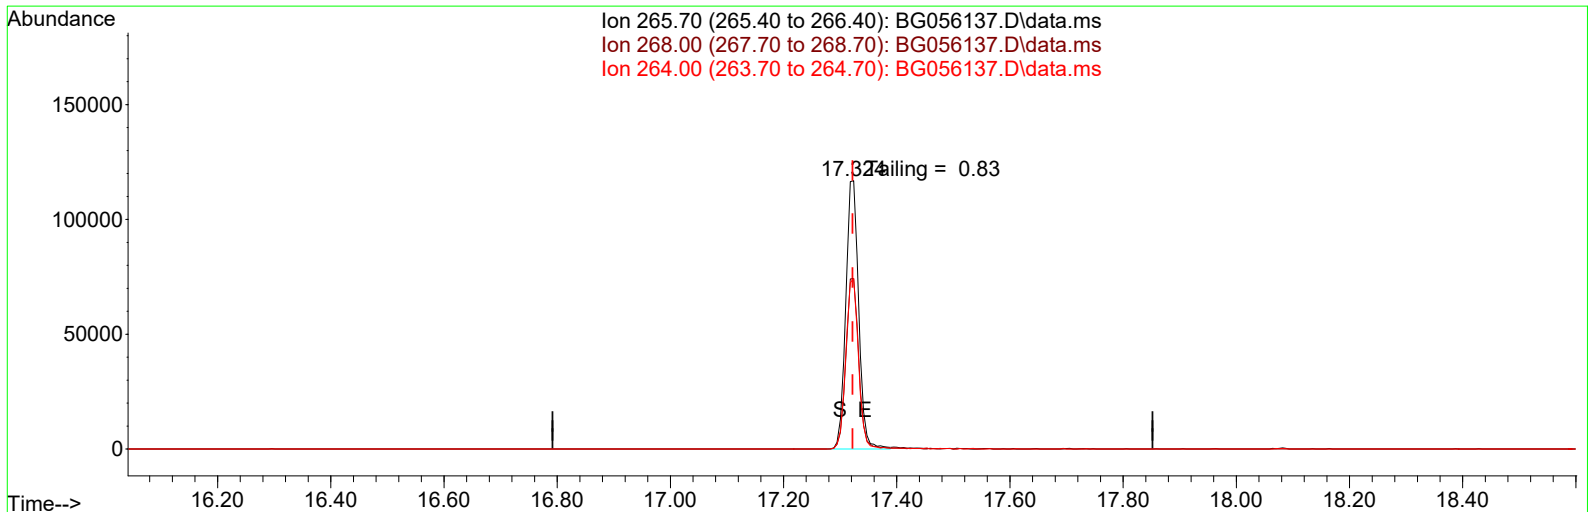

TIC: BG056137.D\data.ms

(70) Pentachlorophenol (C)

17.324min (+ 0.002) 302140.48 ng




response 187504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	63.51
264.00	64.30	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122822\
Data File : BG056137.D
Acq On : 28 Dec 2022 11:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 29 04:58:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

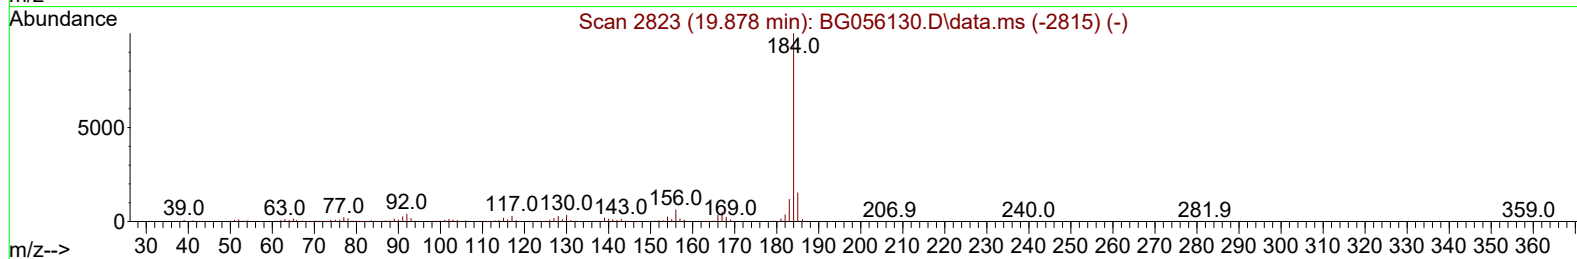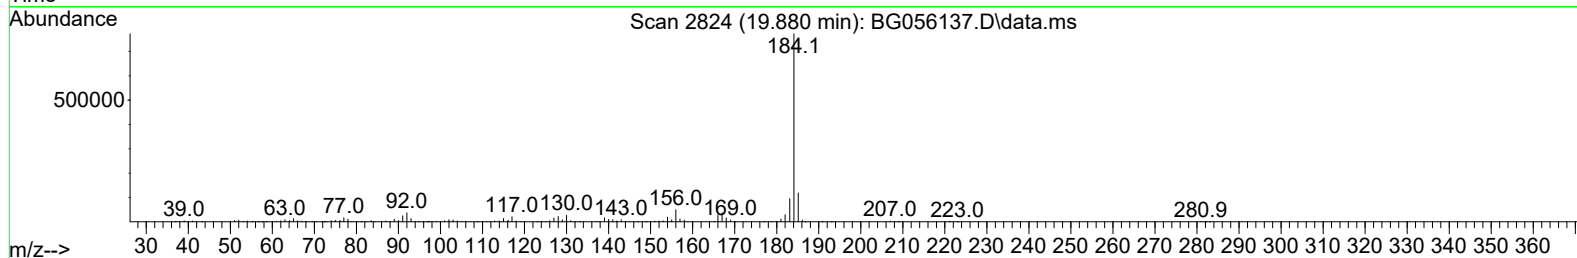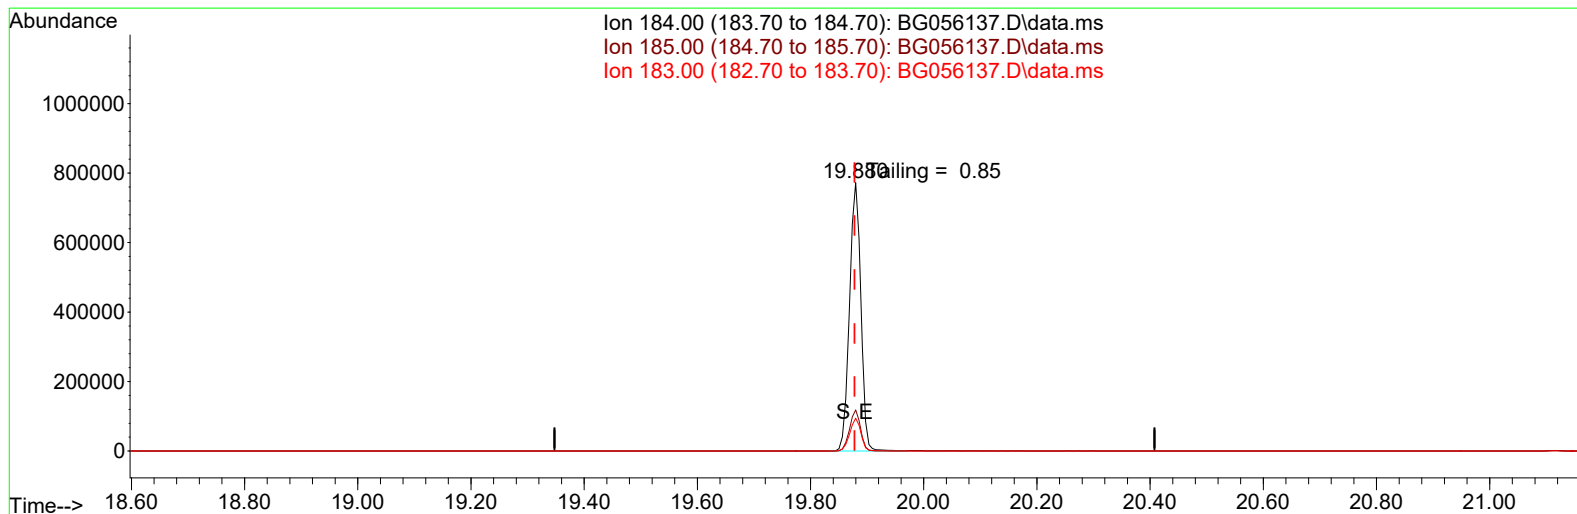

TIC: BG056137.D\data.ms

(77) Benzidine

19.880min (+ 0.002) 393660.62 ng

response 1076054

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.36
183.00	11.70	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2022	BNA_G	BG056137.D
Compound Name	Response	Retention Time
DDT	519196	21.114
DDD	9405	20.655
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9405	528601	1.78

Instrument :
BNA_G
ClientSampleId :
DFTPP