
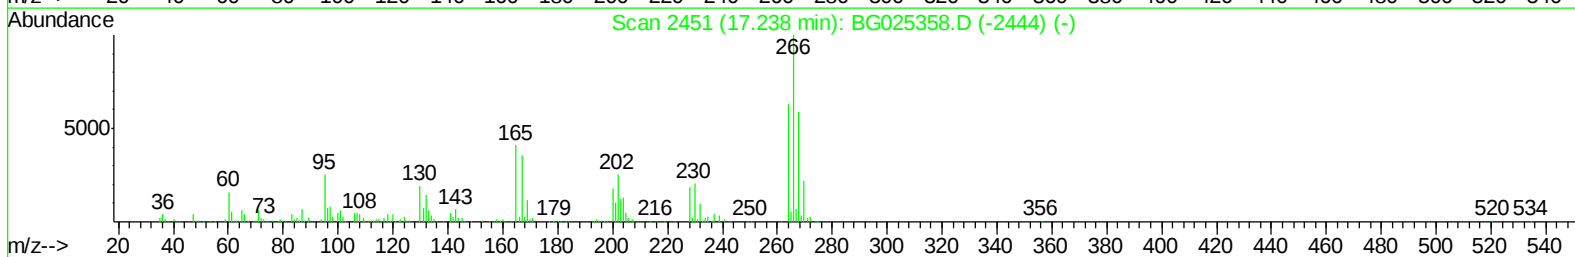
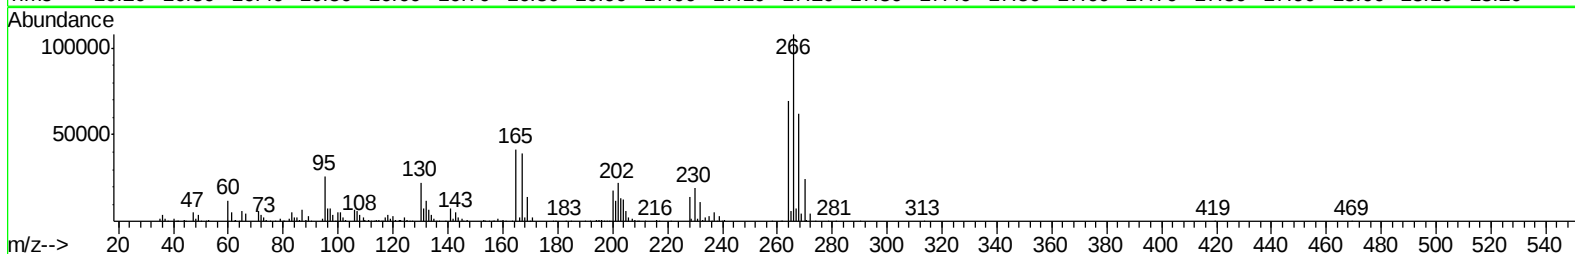


Data Path : Z:\HPCHEM1\BNA_G\Data\BG122916\
Data File : BG025399.D
Acq On : 29 Dec 2016 11:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 06:18:40 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 18:42:01 2016
Response via : Initial Calibration

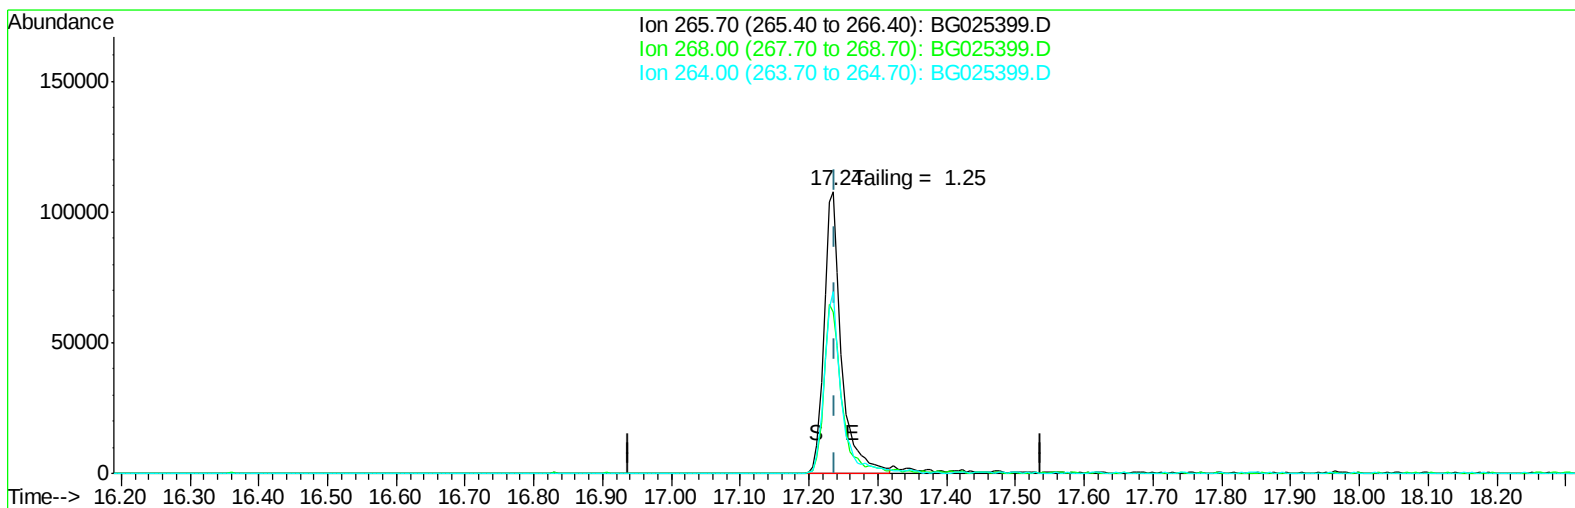

TIC: BG025399.D

(69) Pentachlorophenol (C)




17.235min (-0.003) 153587.71ng

response 190501

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	57.50
264.00	62.60	64.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG122916\
Data File : BG025399.D
Acq On : 29 Dec 2016 11:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 06:18:40 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 18:42:01 2016
Response via : Initial Calibration

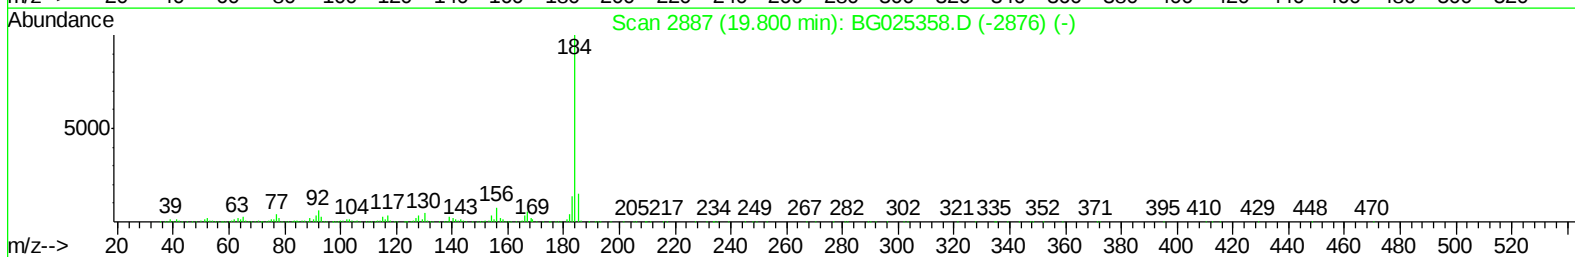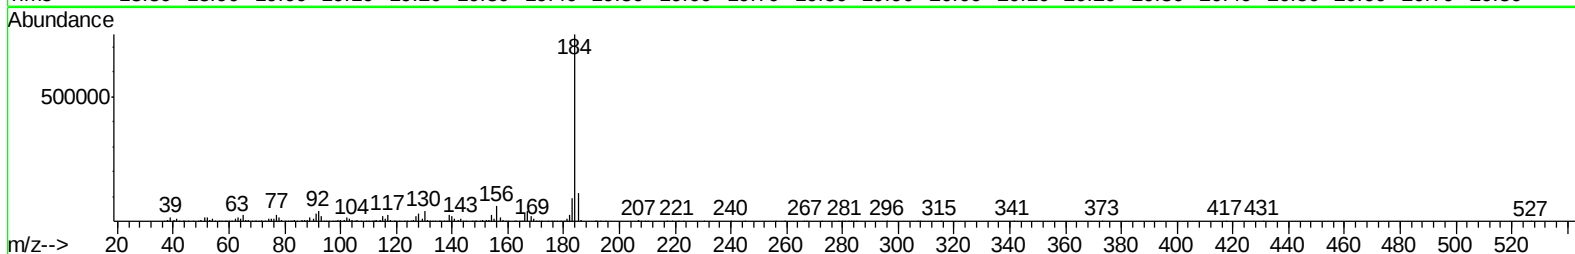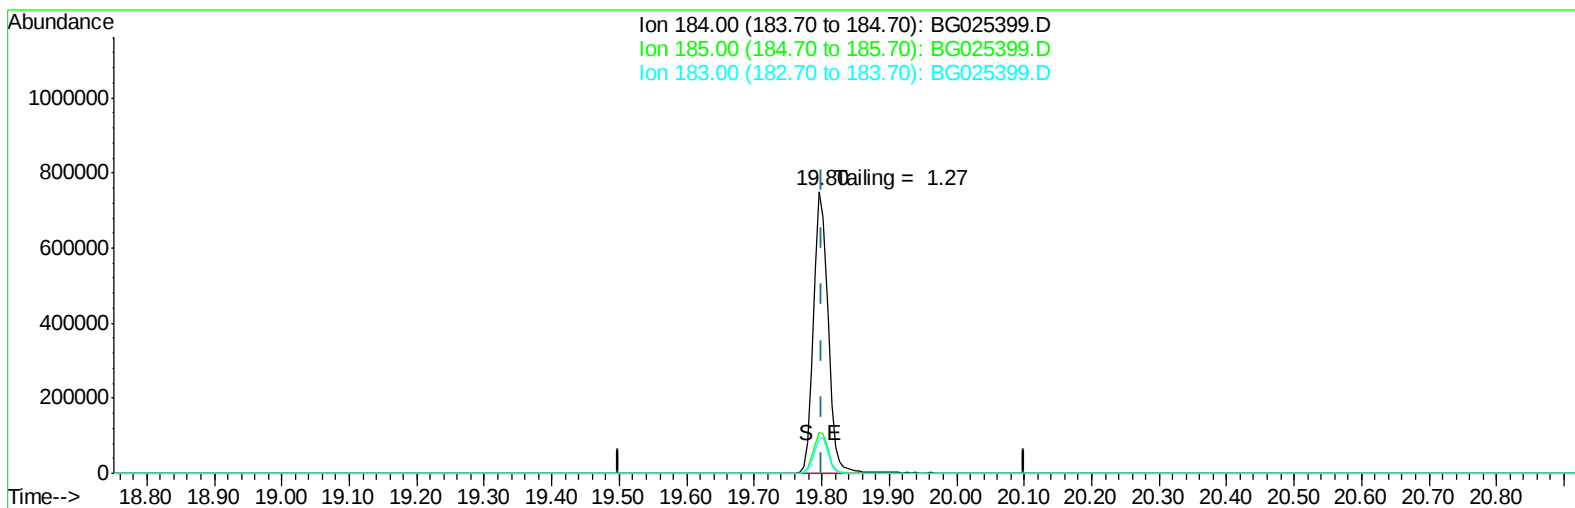

TIC: BG025399.D

(76) Benzidine

19.797min (-0.003) 135501.55ng

response 1112030

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.78
183.00	13.80	12.43
0.00	0.00	0.00