


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122916\
 Data File : BG025399.D
 Acq On : 29 Dec 2016 11:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

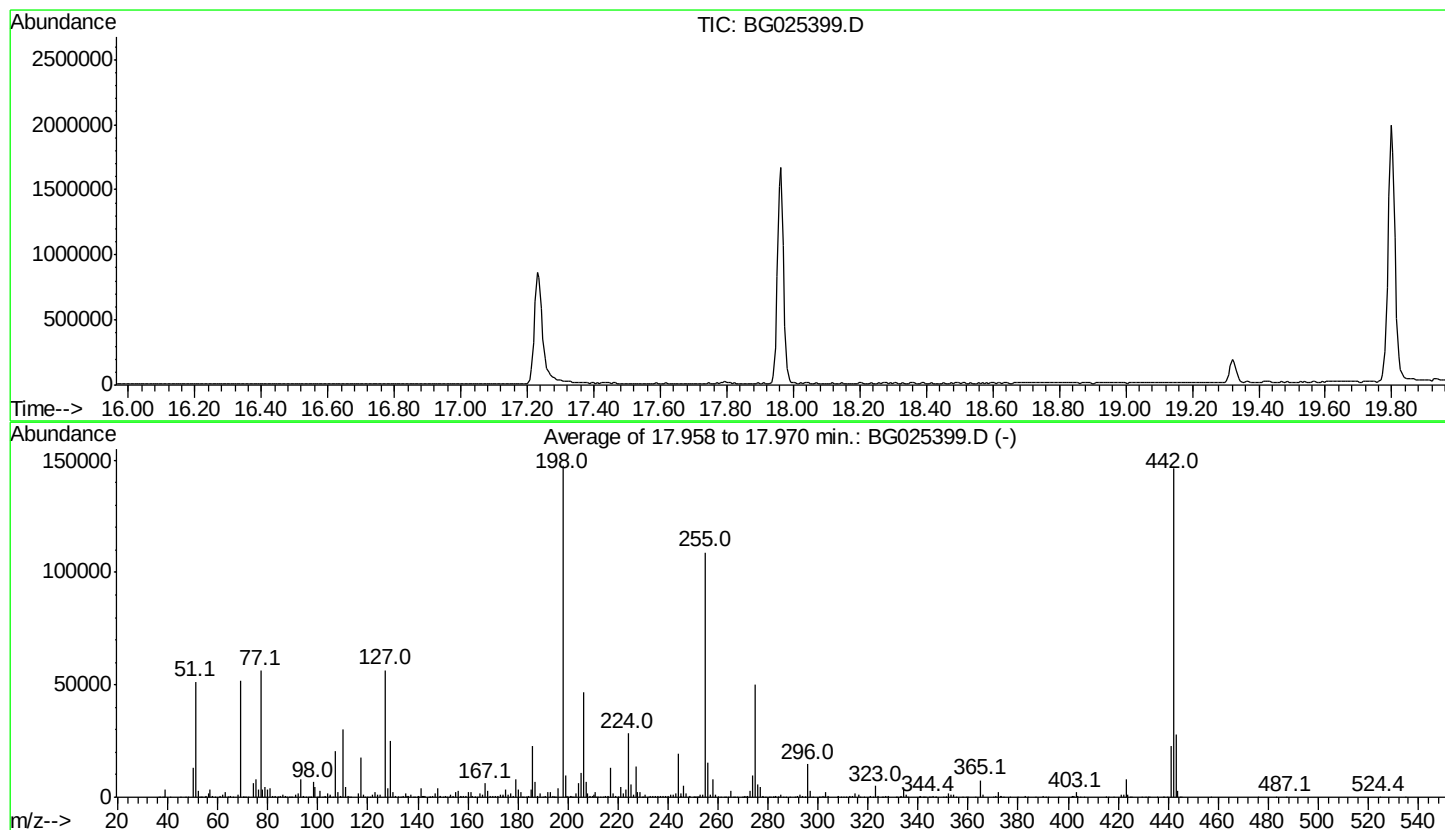

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	51541	PASS
68	69	0.00	2	1.8	945	PASS
69	198	0.00	100	35.0	51589	PASS
70	69	0.00	2	0.2	124	PASS
127	198	10	80	38.2	56400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147536	PASS
199	198	5	9	6.6	9765	PASS
275	198	10	60	33.9	50016	PASS
365	198	1	100	5.1	7572	PASS
441	442	0.01	24	15.5	22738	PASS
442	198	50	100	99.2	146282	PASS
443	442	15	24	19.0	27826	PASS