
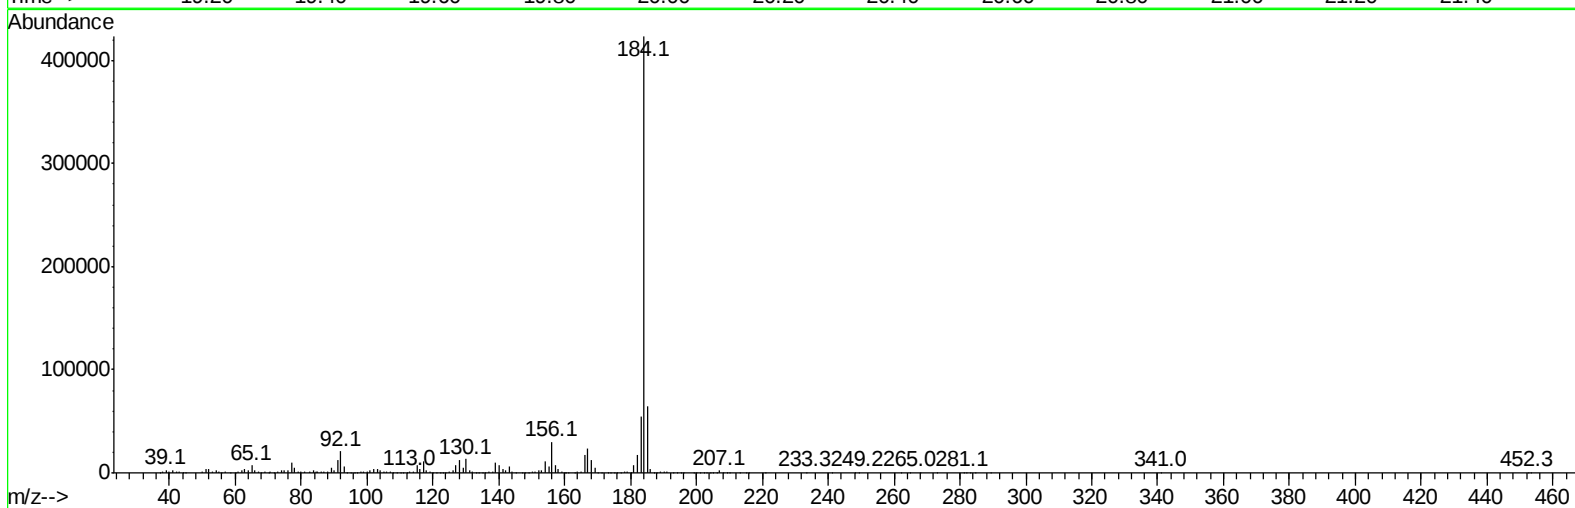


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122917\
Data File : BG031851.D
Acq On : 29 Dec 2017 13:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 23:59:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

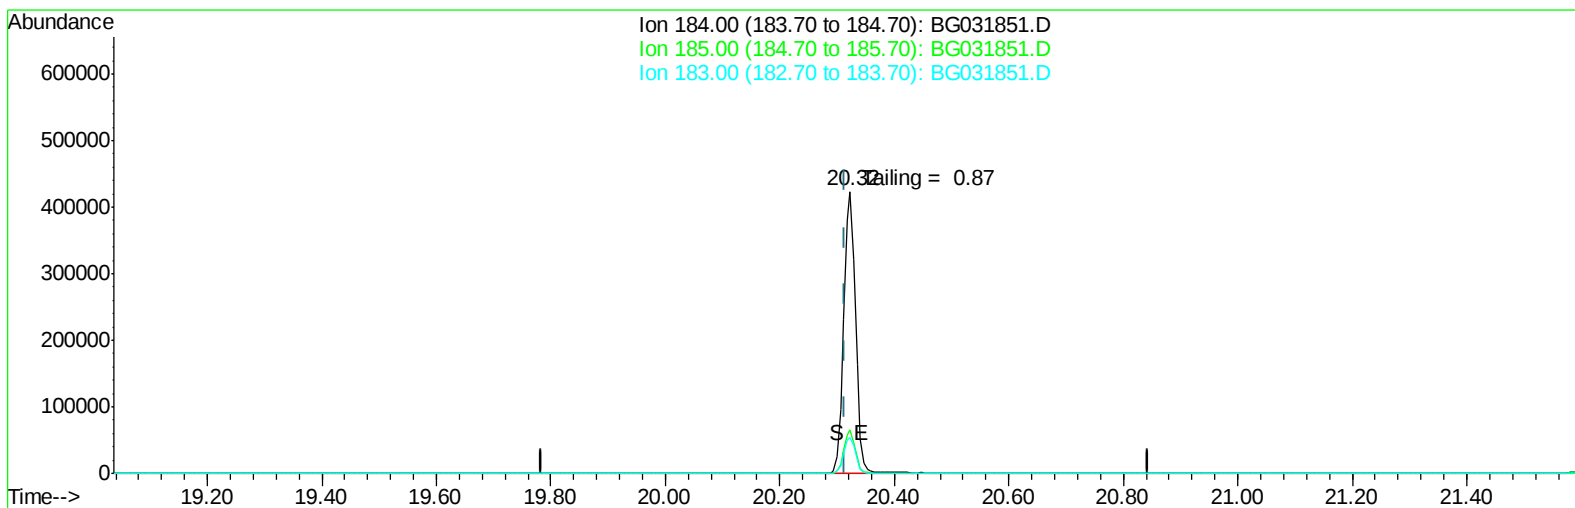

TIC: BG031851.D

(76) Benzidine



20.323min (+0.009) 331706.54ng

response 614295

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.29
183.00	13.30	12.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122917\
Data File : BG031851.D
Acq On : 29 Dec 2017 13:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 23:59:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

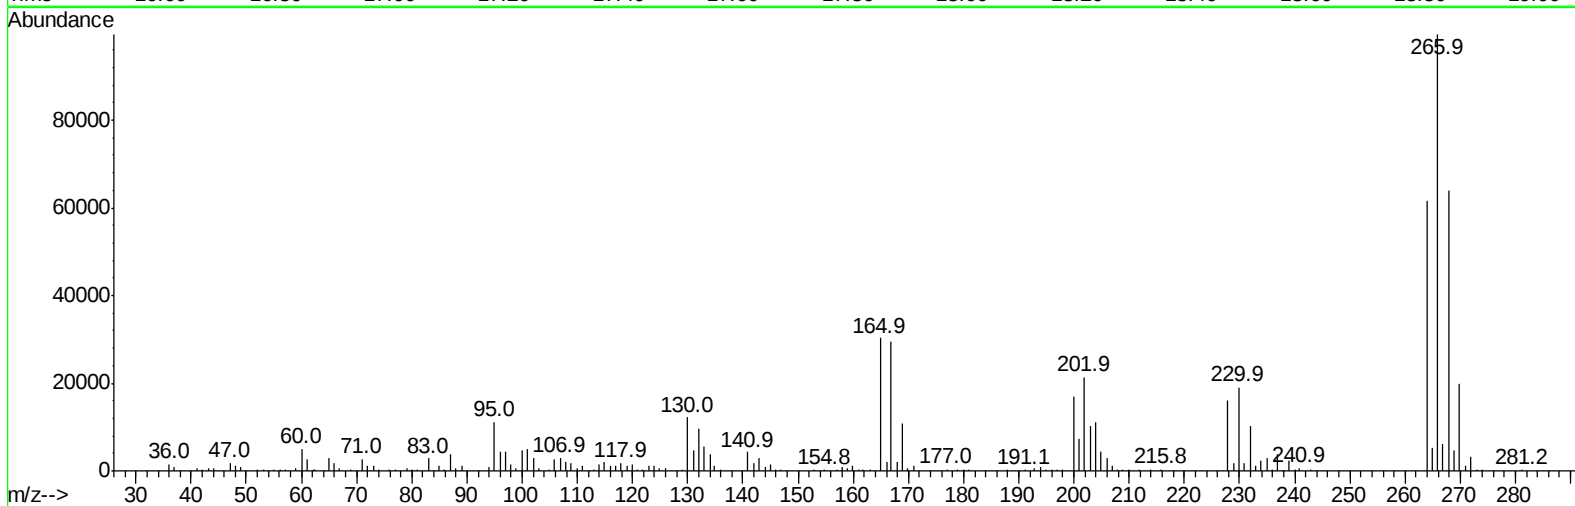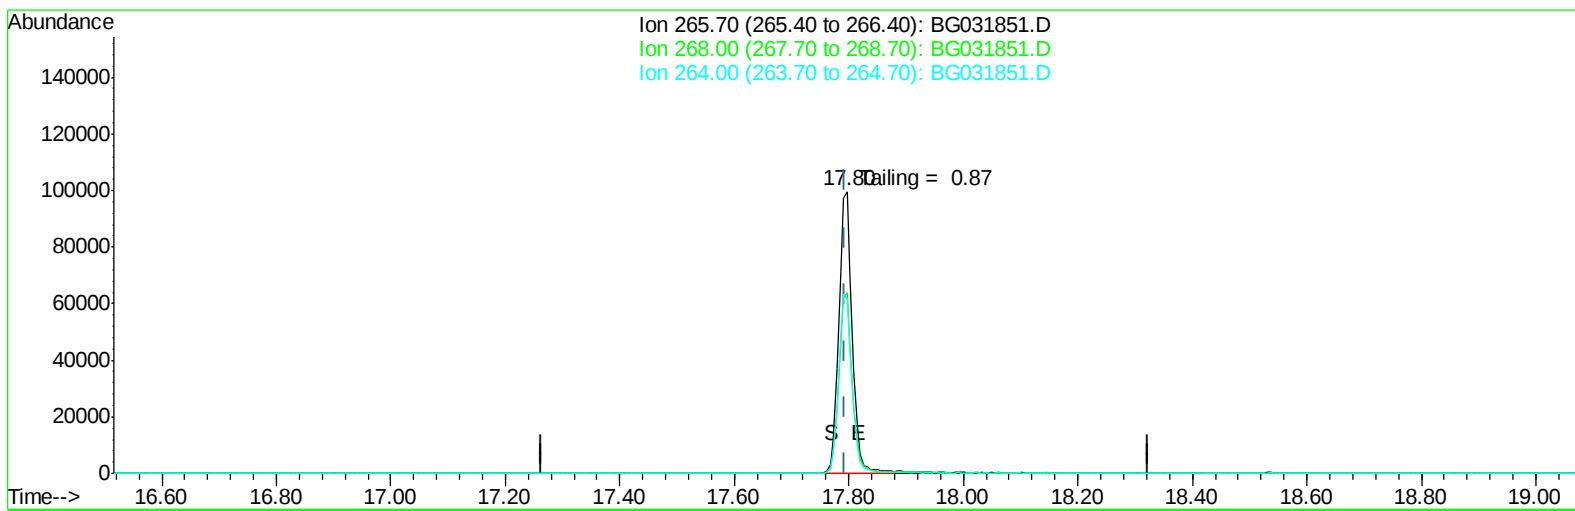

TIC: BG031851.D

(69) Pentachlorophenol (C)

17.797min (+0.003) 243786.68ng

response 163598

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.10
264.00	62.00	61.99
0.00	0.00	0.00