


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122917\
 Data File : BG031851.D
 Acq On : 29 Dec 2017 13:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 15:51:46 2017

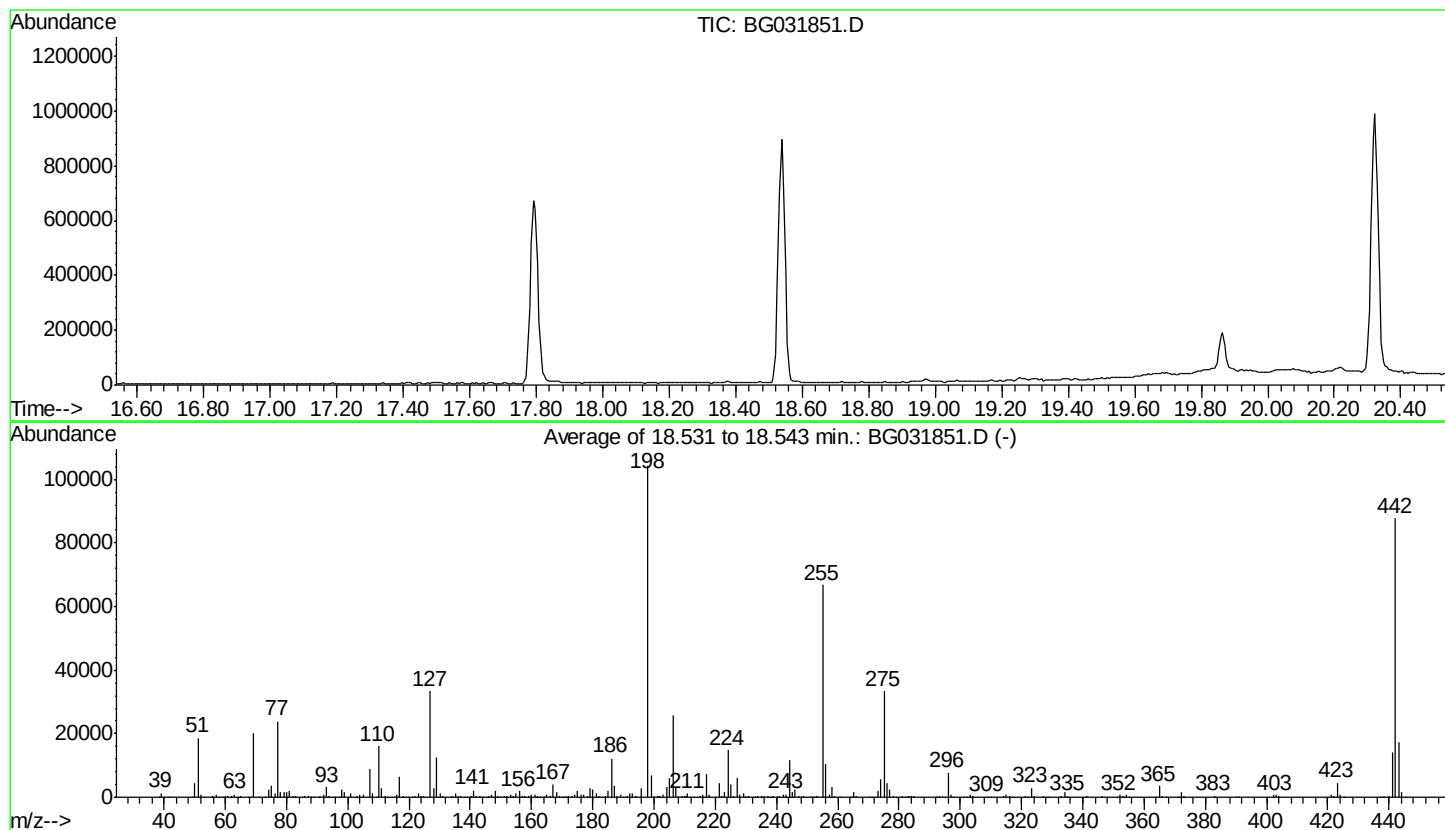

AutoFind: Scans 2594, 2595, 2596; Background Corrected with Scan 2587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.9	18698	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.4	20197	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.9	33317	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104349	PASS
199	198	5	9	6.6	6865	PASS
275	198	10	60	32.0	33400	PASS
365	198	1	100	3.4	3565	PASS
441	442	0.01	24	16.2	14229	PASS
442	198	50	100	84.0	87704	PASS
443	442	15	24	19.8	17396	PASS