
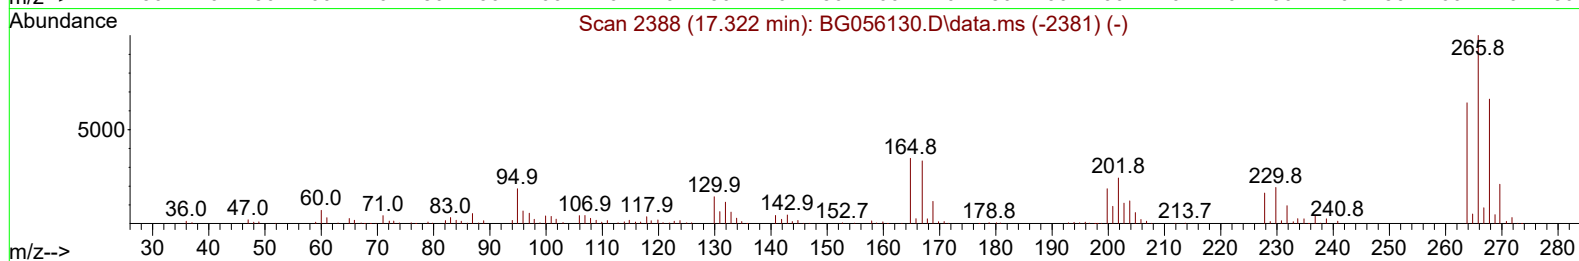
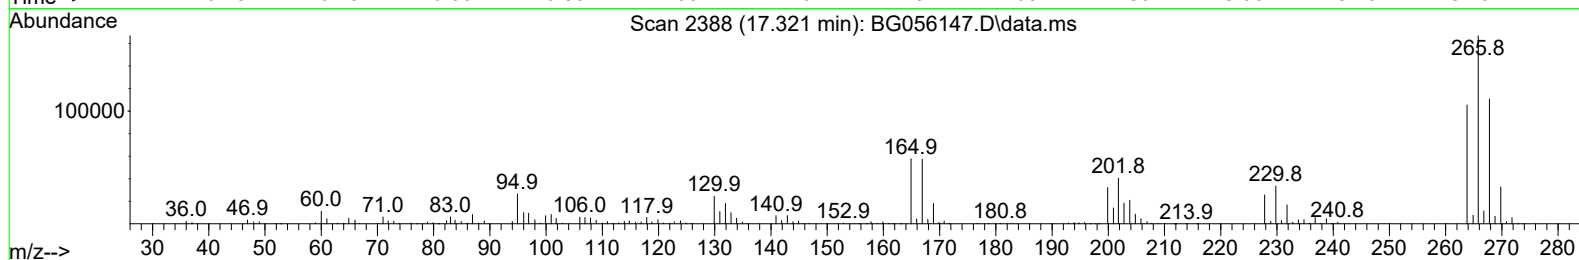


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122922\
Data File : BG056147.D
Acq On : 29 Dec 2022 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 04:44:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

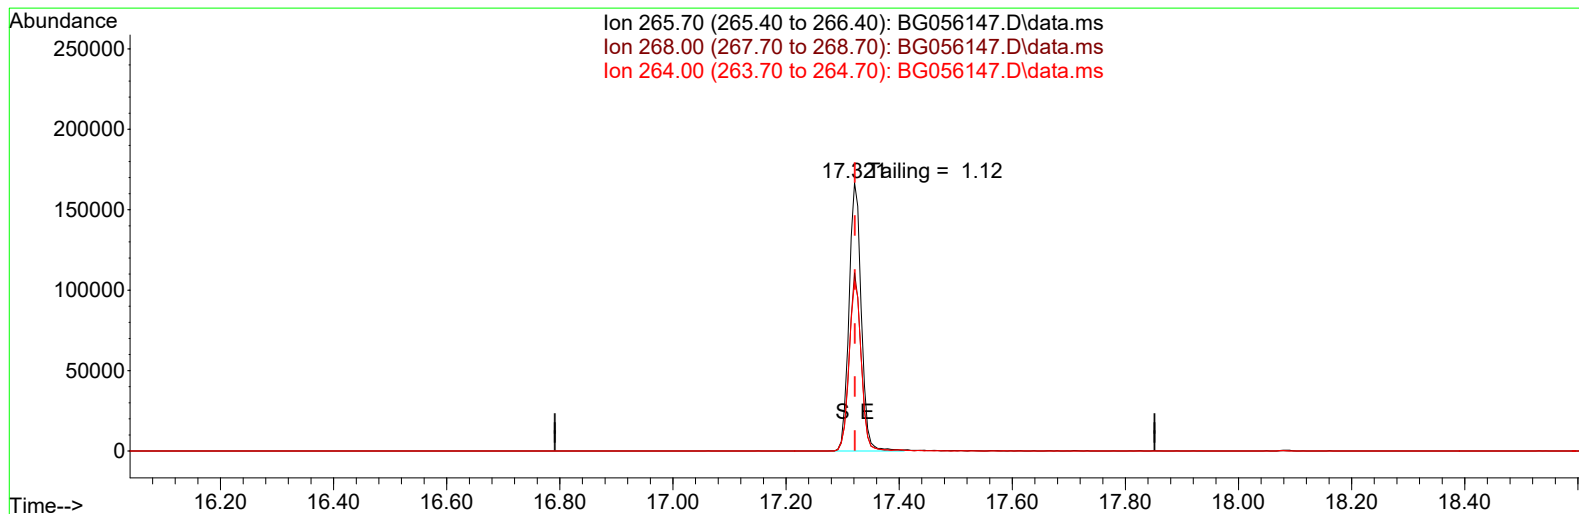

TIC: BG056147.D\data.ms

(70) Pentachlorophenol (C)




17.321min (-0.001) 285065.09 ng

response 252353

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.39
264.00	64.30	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122922\
Data File : BG056147.D
Acq On : 29 Dec 2022 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 04:44:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

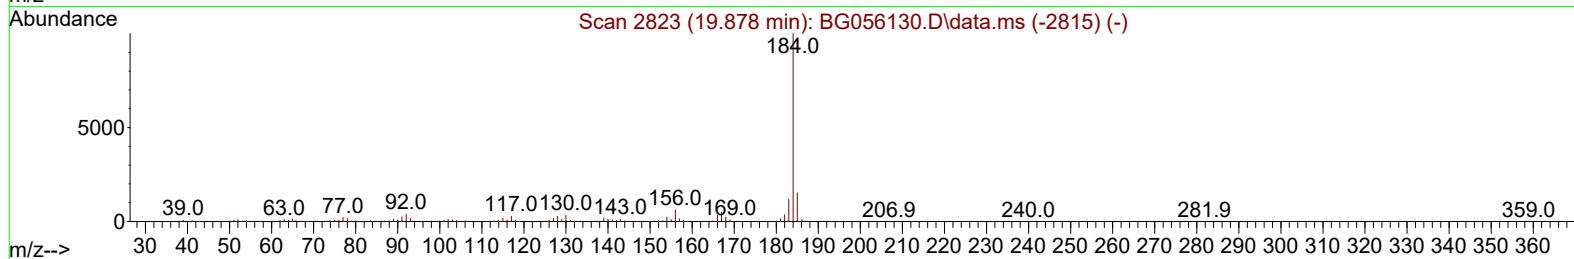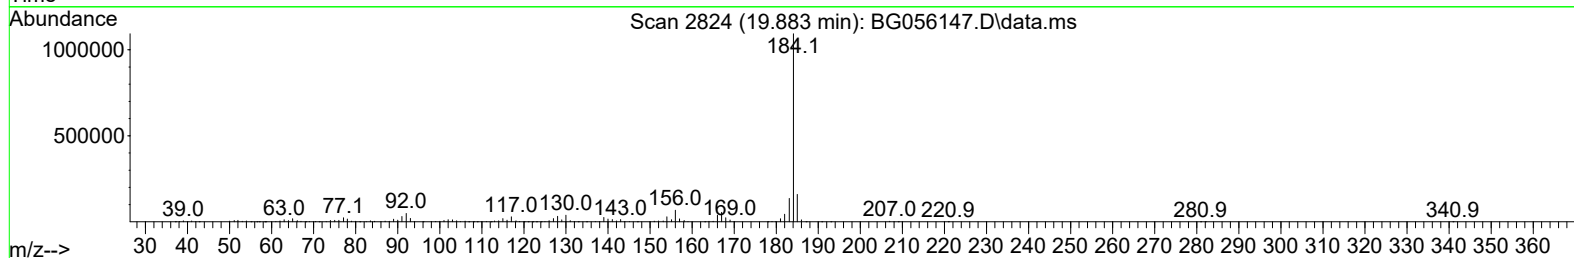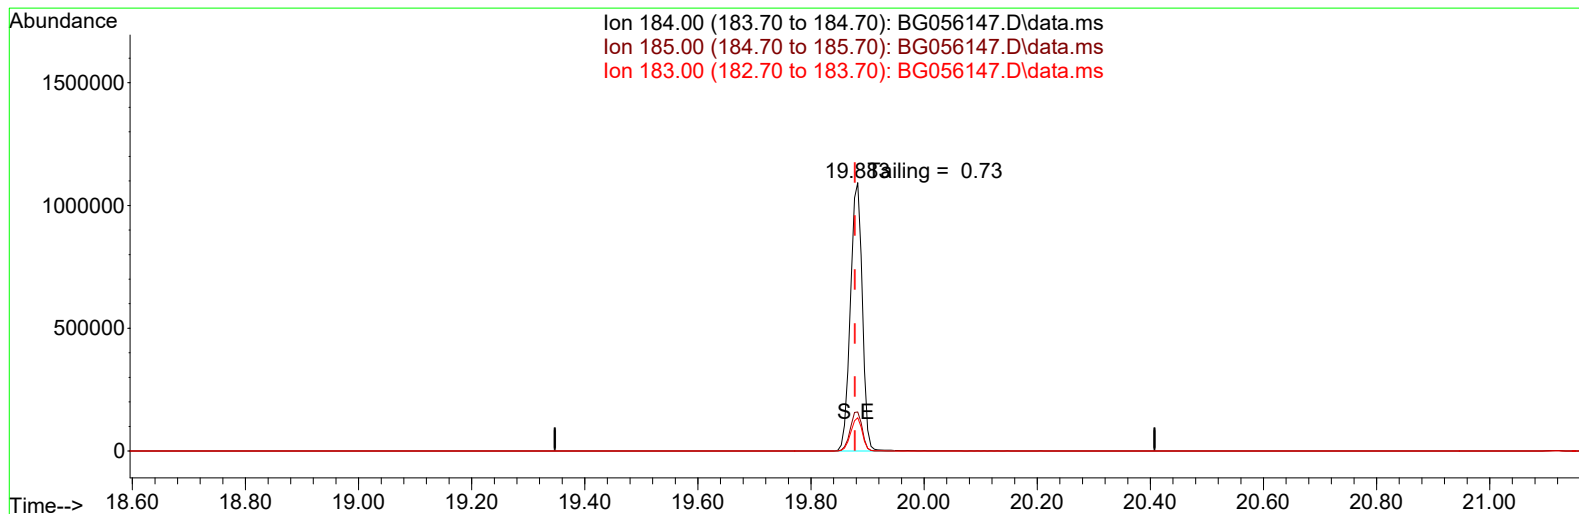

TIC: BG056147.D\data.ms

(77) Benzidine

19.883min (+ 0.005) 4083.42 ng m

response 1597862

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.58
183.00	11.70	12.44
0.00	0.00	0.00