
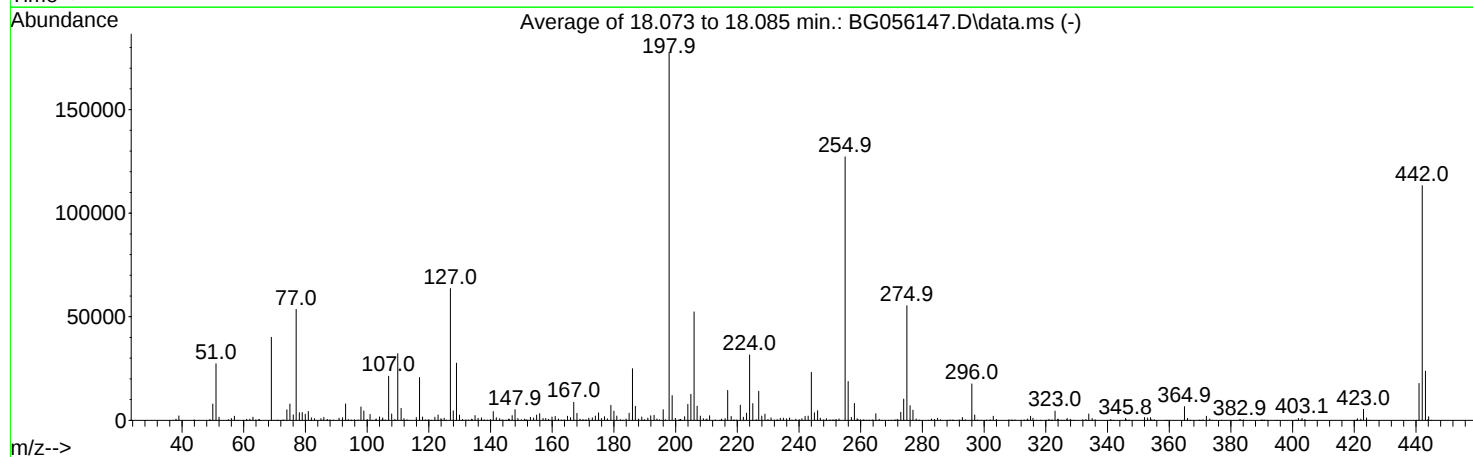


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122922\
 Data File : BG056147.D
 Acq On : 29 Dec 2022 9:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 05:20:14 2022

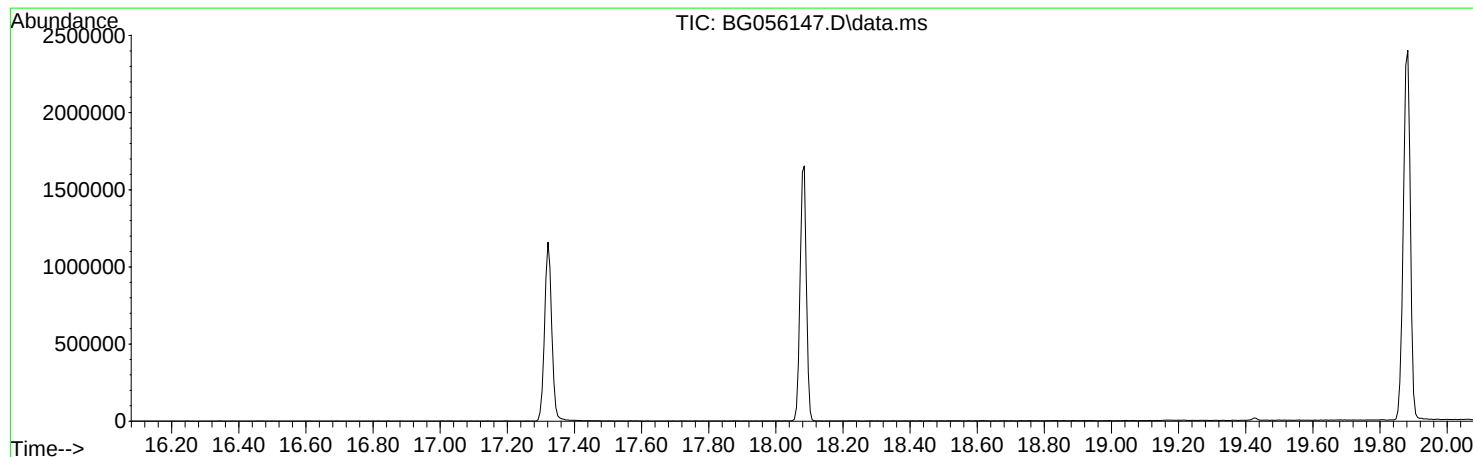




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.4	27325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.6	40091	PASS
70	69	0.00	2	0.2	76	PASS
127	198	10	80	35.8	63597	PASS
197	198	0.00	2	0.1	264	PASS
198	198	100	100	100.0	177613	PASS
199	198	5	9	6.7	11917	PASS
275	198	10	60	31.1	55320	PASS
365	198	1	100	3.7	6647	PASS
441	198	0.01	100	10.0	17814	PASS
442	442	50	100	100.0	113280	PASS
443	442	15	24	20.9	23720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122922\
Data File : BG056147.D
Acq On : 29 Dec 2022 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 30 04:44:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

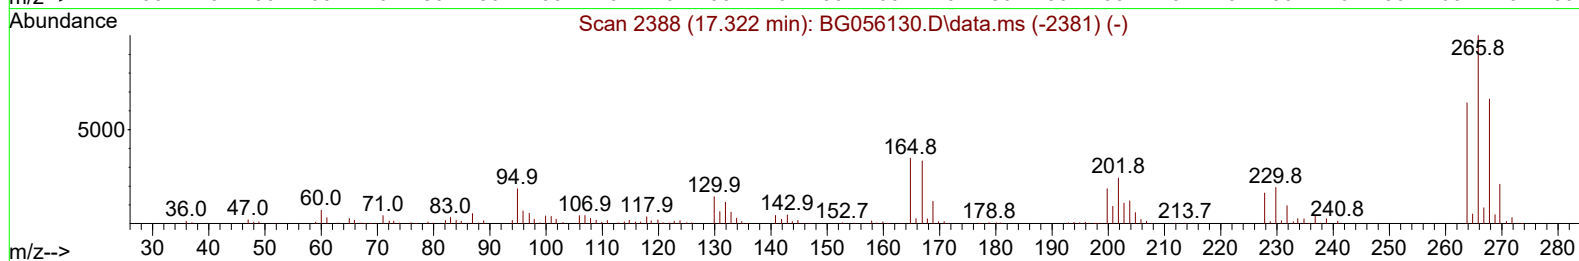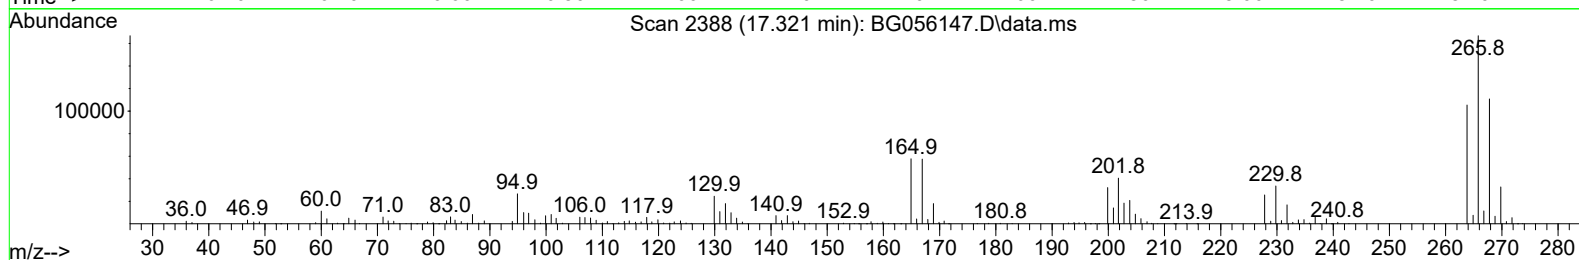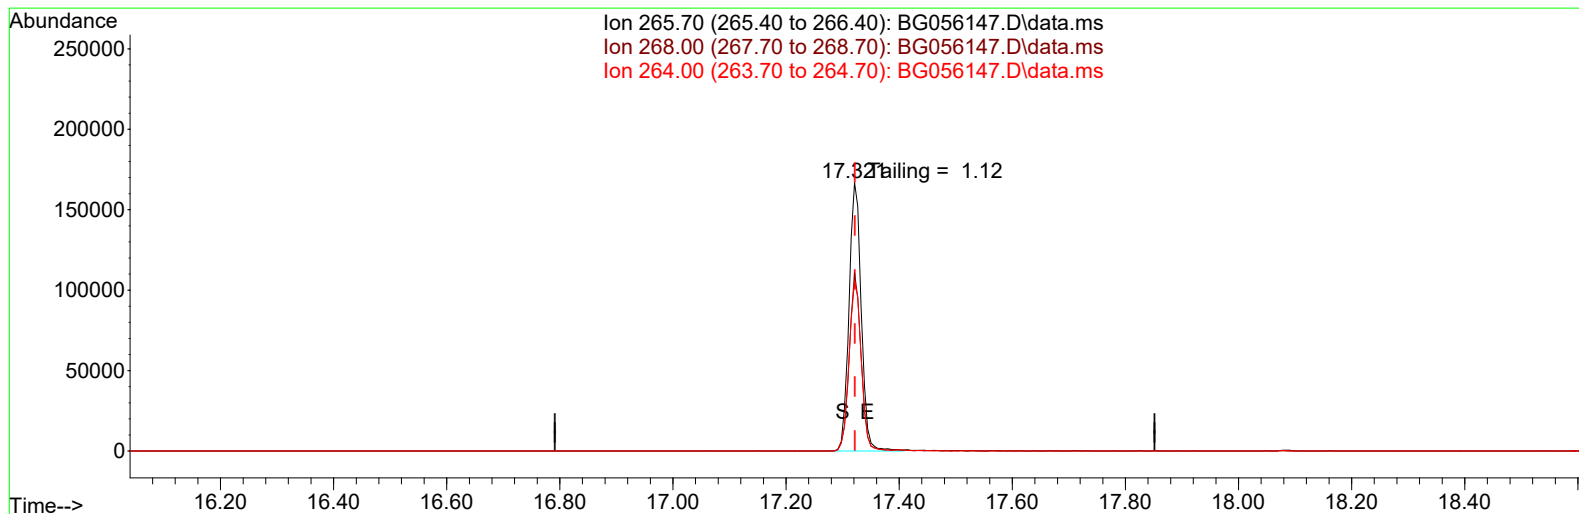

TIC: BG056147.D\data.ms

(70) Pentachlorophenol (C)

17.321min (-0.001) 285065.09 ng




response 252353

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.39
264.00	64.30	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122922\
Data File : BG056147.D
Acq On : 29 Dec 2022 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 30 04:44:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

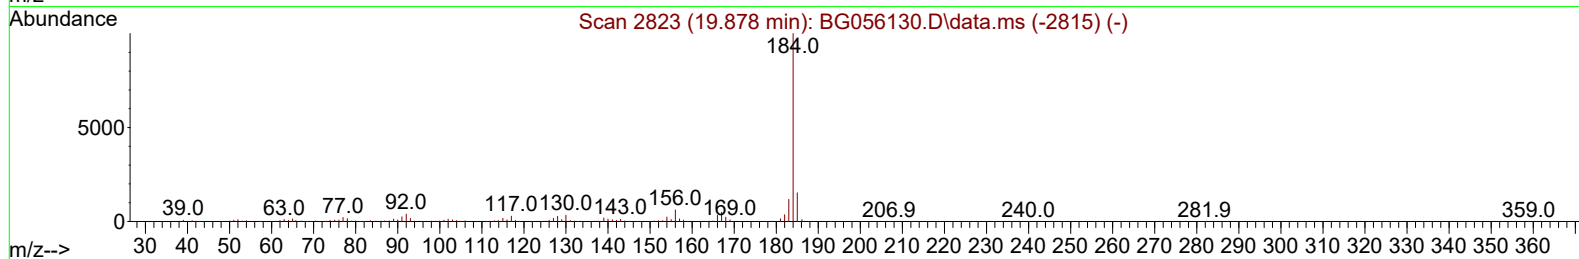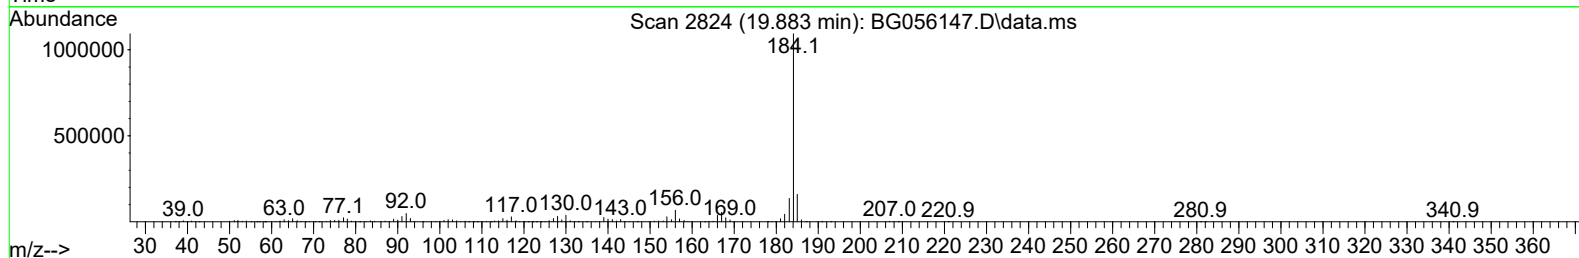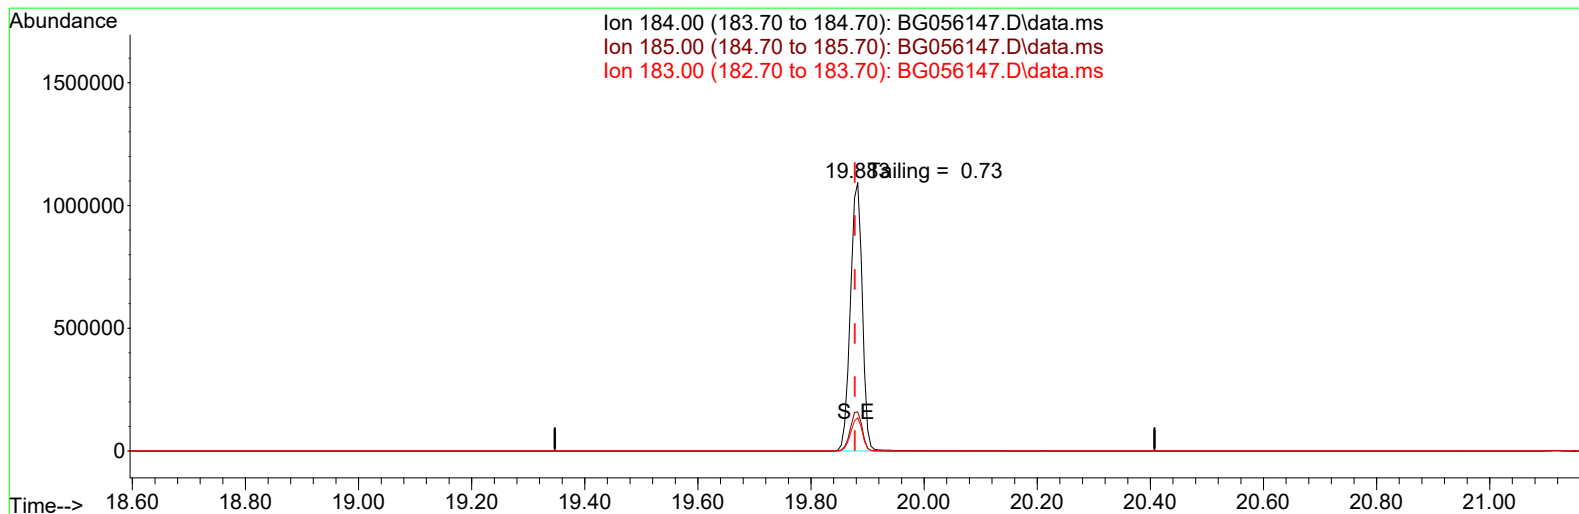

TIC: BG056147.D\data.ms

(77) Benzidine

19.883min (+ 0.005) 4083.42 ng m

response 1597862

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.58
183.00	11.70	12.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/29/2022	BNA_G	BG056147.D
Compound Name	Response	Retention Time
DDT	758800	21.116
DDD	11379	20.711
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11379	770179	1.48

Instrument :
BNA_G
ClientSampleId :
DFTPP