

Data Path : Z:\HPCHEM1\BNA G\DATA\BG123015\
 Data File : BG020605.D
 Acq On : 30 Dec 2015 12:39
 Operator : UM/SJ
 Sample : G4803-02RX
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04C2RX

Quant Time: Dec 30 15:56:33 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG123015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 30 08:00:55 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	15476	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	72669	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.69	164	57737	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.44	188	155784	20.00	ng/ul	0.00
78) Chrysene-d12	21.71	240	185580	20.00	ng/ul	0.00
86) Perylene-d12	24.96	264	178851	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.23	99	2143	1.64	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.38	67	5618	7.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.59	132	6433	6.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.77	113	4385	3.91	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	4047	7.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	4803	7.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.50	165	8907	7.20	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.10	166	43034	9.11	ng/ul	0.00
47) Acenaphthylene-d8	14.39	160	42775	7.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	288	0.39	ng/ul	0.02
58) Fluorene-d10	15.69	176	36830	8.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	5888	6.23	ng/ul	0.00
71) Anthracene-d10	17.54	188	67762	9.34	ng/ul	0.00
79) Pyrene-d10	19.82	212	83433	10.02	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.74	264	82514	9.25	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.14	163	29519	6.11	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG123015\
Data File : BG020605.D
Acq On : 30 Dec 2015 12:39
Operator : UM/SJ
Sample : G4803-02RX
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04C2RX

Quant Time: Dec 30 15:56:33 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG123015.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 30 08:00:55 2015
Response via : Initial Calibration

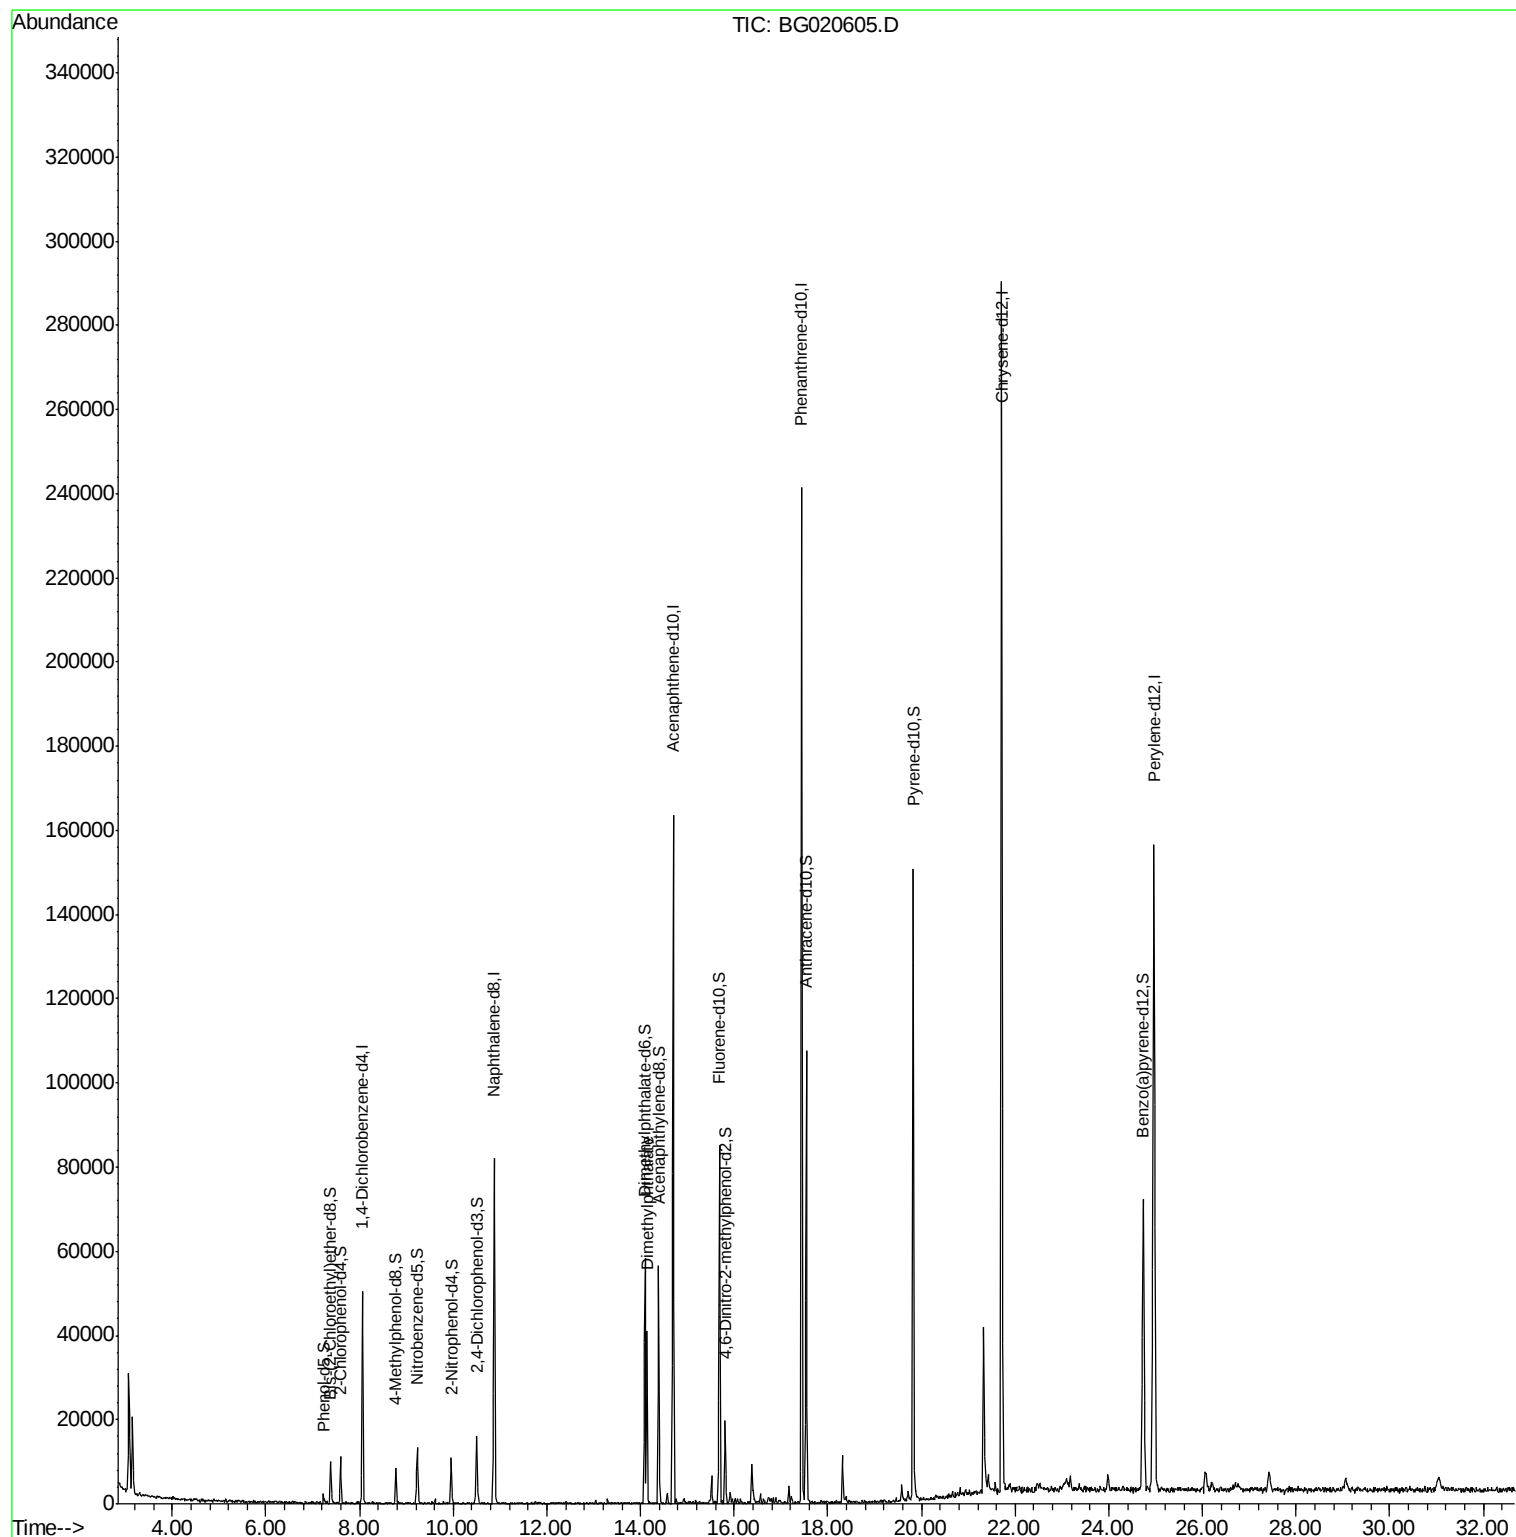

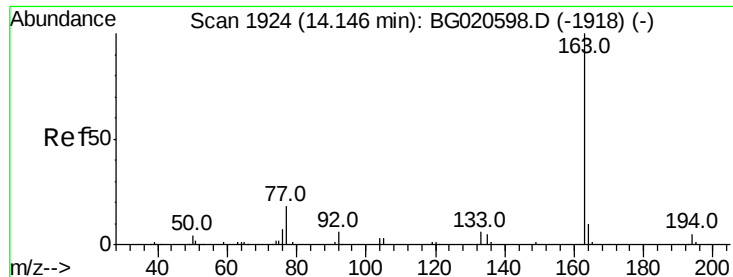

#45

Dimethylphthalate

Concen: 6.11 ng/ul

RT: 14.14 min Scan# 1924

Delta R.T. -0.00 min

Lab File: BG020605.D

Acq: 30 Dec 2015 12:39

Instrument :

BNA_G

ClientSampleId :

C04C2RX


Tot Ion:163 Resp: 29519

Ion Ratio Lower Upper

163 100

194 4.9 4.0 6.0

164 9.1 8.4 12.6

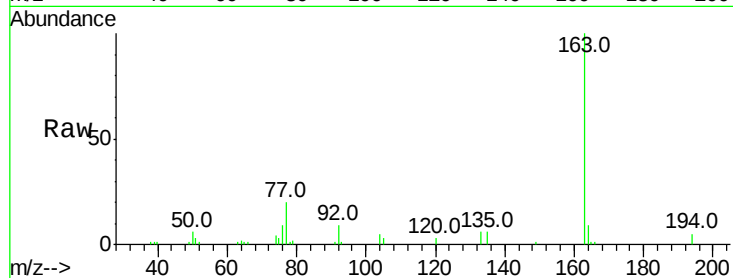

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

